


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE032619\
 Data File : BE099218.D
 Acq On : 26 Mar 2019 16:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 26 07:02:06 2019

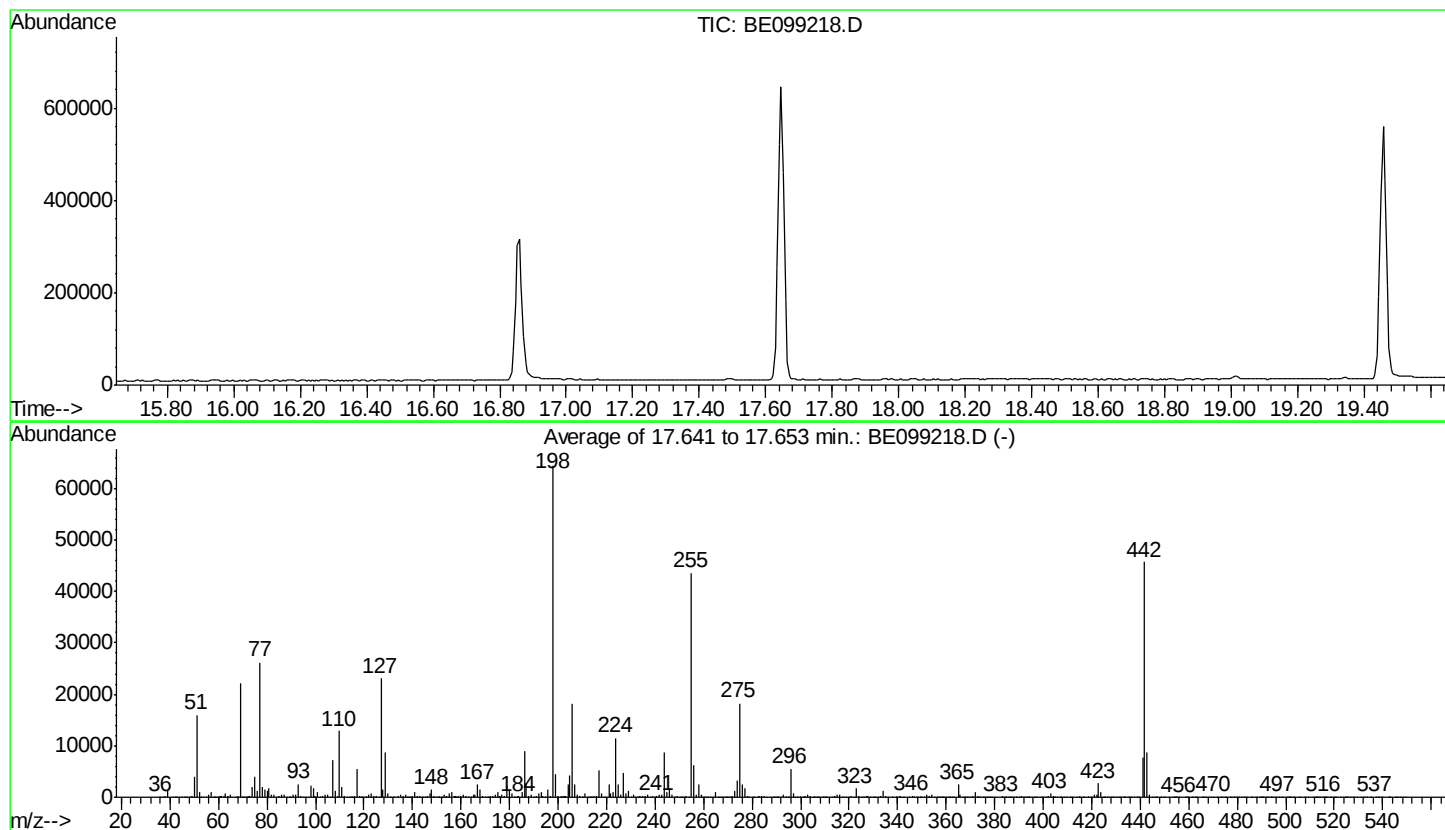

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.8	15944	PASS
68	69	0.00	2	1.5	335	PASS
69	198	0.00	100	34.4	22136	PASS
70	69	0.00	2	0.4	81	PASS
127	198	10	80	35.9	23112	PASS
197	198	0.00	2	0.3	176	PASS
198	198	100	100	100.0	64414	PASS
199	198	5	9	6.8	4360	PASS
275	198	10	60	28.2	18173	PASS
365	198	1	100	3.7	2380	PASS
441	198	0.01	100	12.1	7773	PASS
442	198	50	100	70.9	45672	PASS
443	442	15	24	18.9	8654	PASS