


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE032619\
 Data File : BE099237.D
 Acq On : 27 Mar 2019 6:12
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 26 07:02:06 2019

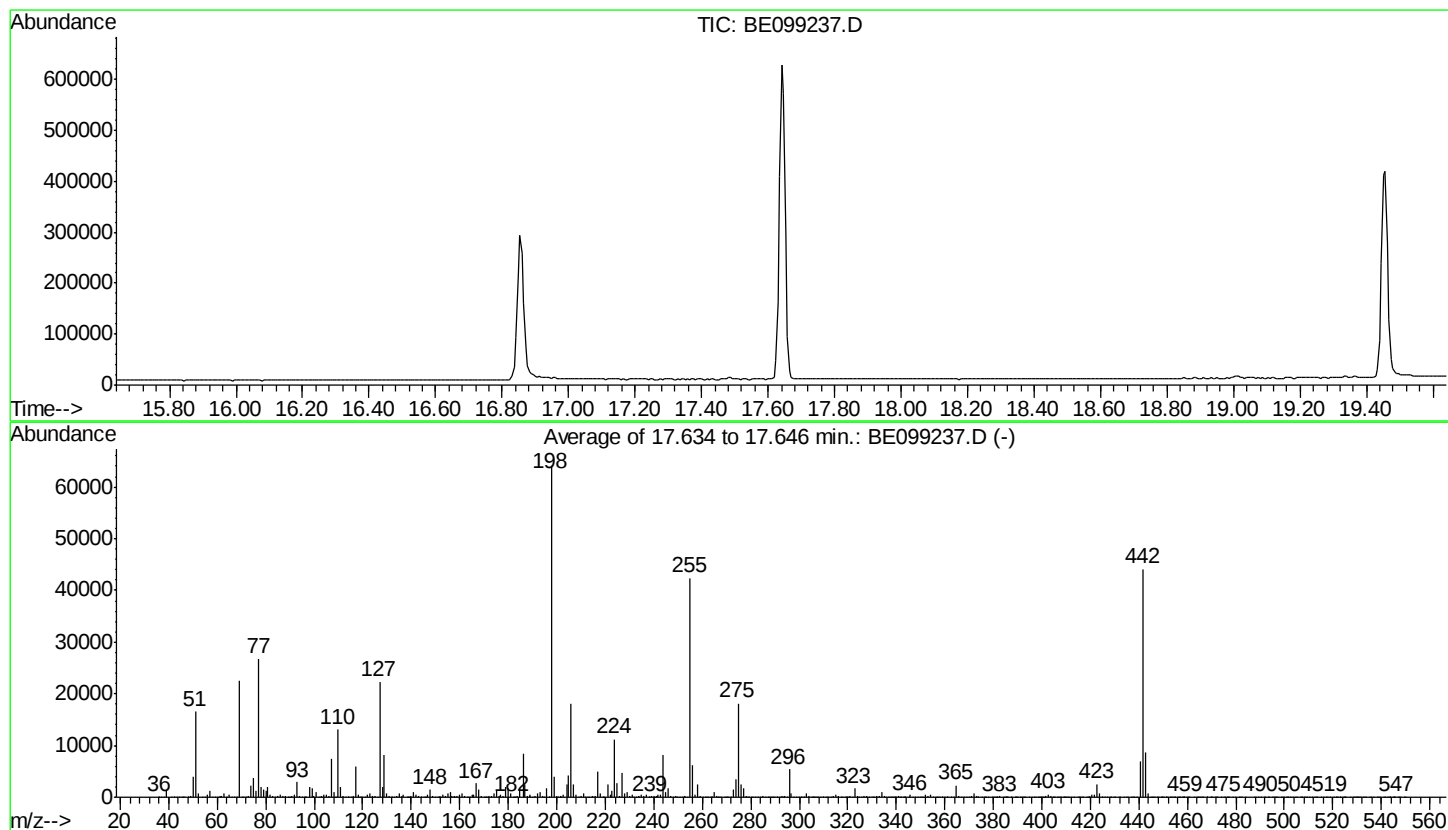

AutoFind: Scans 2561, 2562, 2563; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.8	16550	PASS
68	69	0.00	2	0.3	66	PASS
69	198	0.00	100	35.3	22628	PASS
70	69	0.00	2	0.6	129	PASS
127	198	10	80	34.9	22377	PASS
197	198	0.00	2	0.2	118	PASS
198	198	100	100	100.0	64125	PASS
199	198	5	9	6.4	4079	PASS
275	198	10	60	28.4	18180	PASS
365	198	1	100	3.6	2316	PASS
441	198	0.01	100	10.7	6884	PASS
442	198	50	100	68.8	44118	PASS
443	442	15	24	19.9	8786	PASS