


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE040219\
 Data File : BE099269.D
 Acq On : 2 Apr 2019 11:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE040219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 02 17:16:42 2019

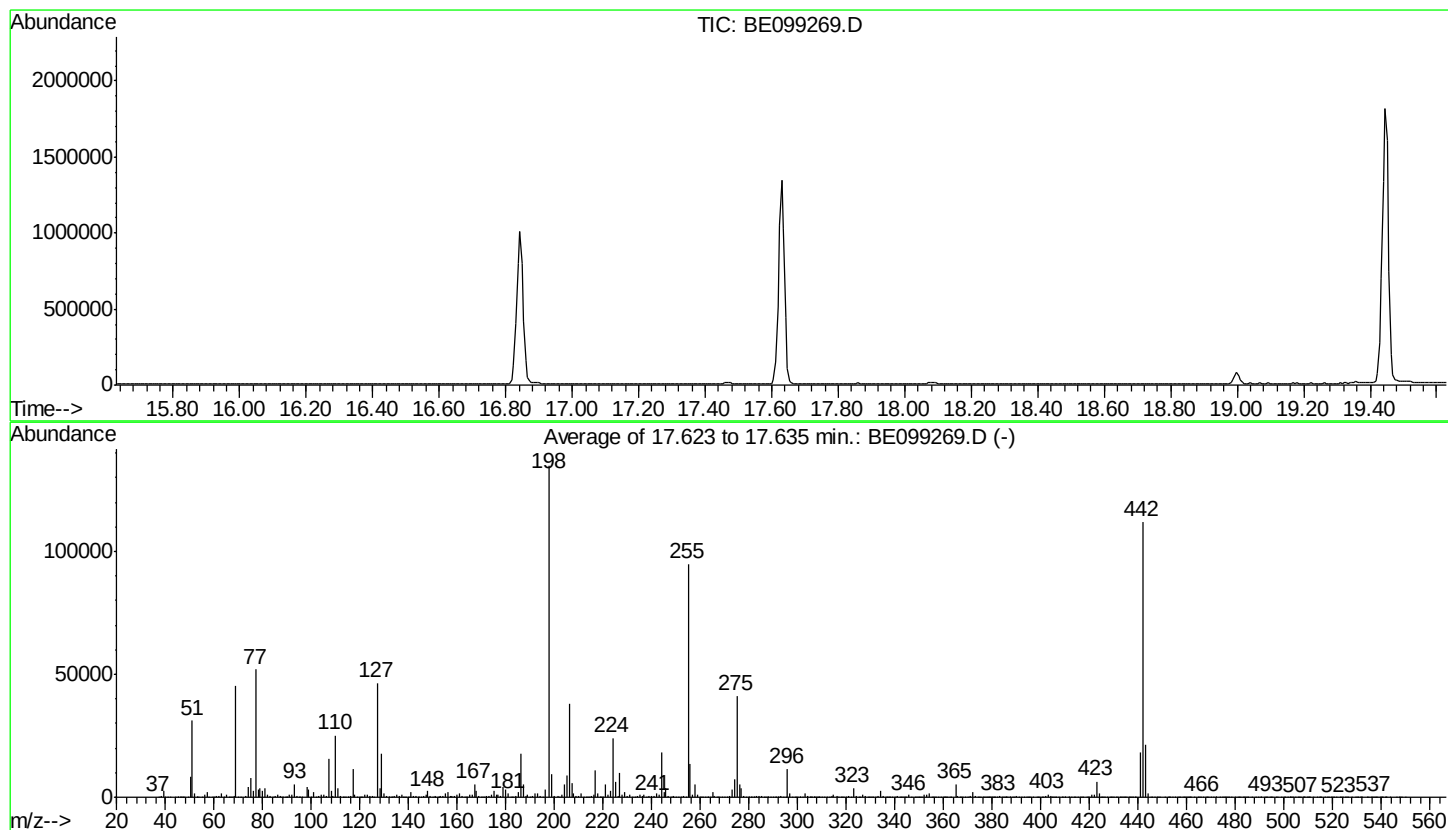

AutoFind: Scans 2559, 2560, 2561; Background Corrected with Scan 2552

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.1	31148	PASS
68	69	0.00	2	1.2	537	PASS
69	198	0.00	100	33.8	45572	PASS
70	69	0.00	2	0.4	181	PASS
127	198	10	80	34.5	46530	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	134883	PASS
199	198	5	9	7.1	9541	PASS
275	198	10	60	30.6	41325	PASS
365	198	1	100	3.9	5251	PASS
441	198	0.01	100	13.4	18132	PASS
442	198	50	100	83.0	112003	PASS
443	442	15	24	19.3	21592	PASS