
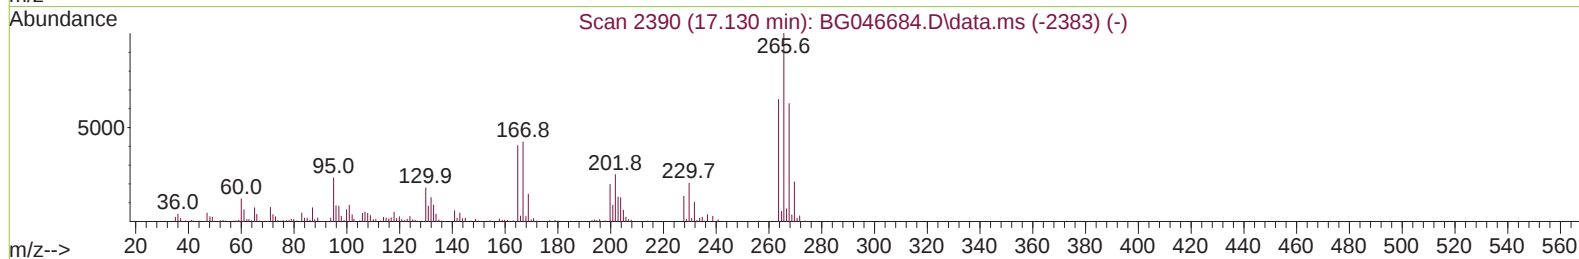
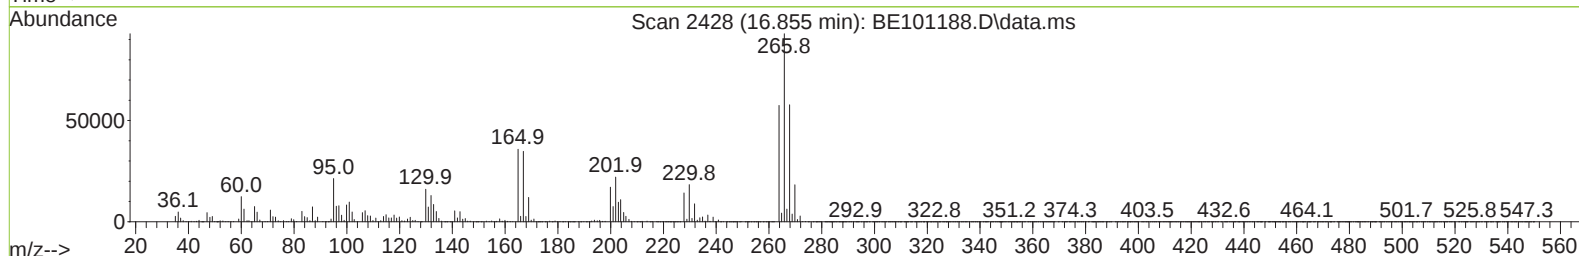


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040221\
 Data File : BE101188.D
 Acq On : 2 Apr 2021 7:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 09:26:35 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 31 10:54:22 2021
 Response via : Initial Calibration

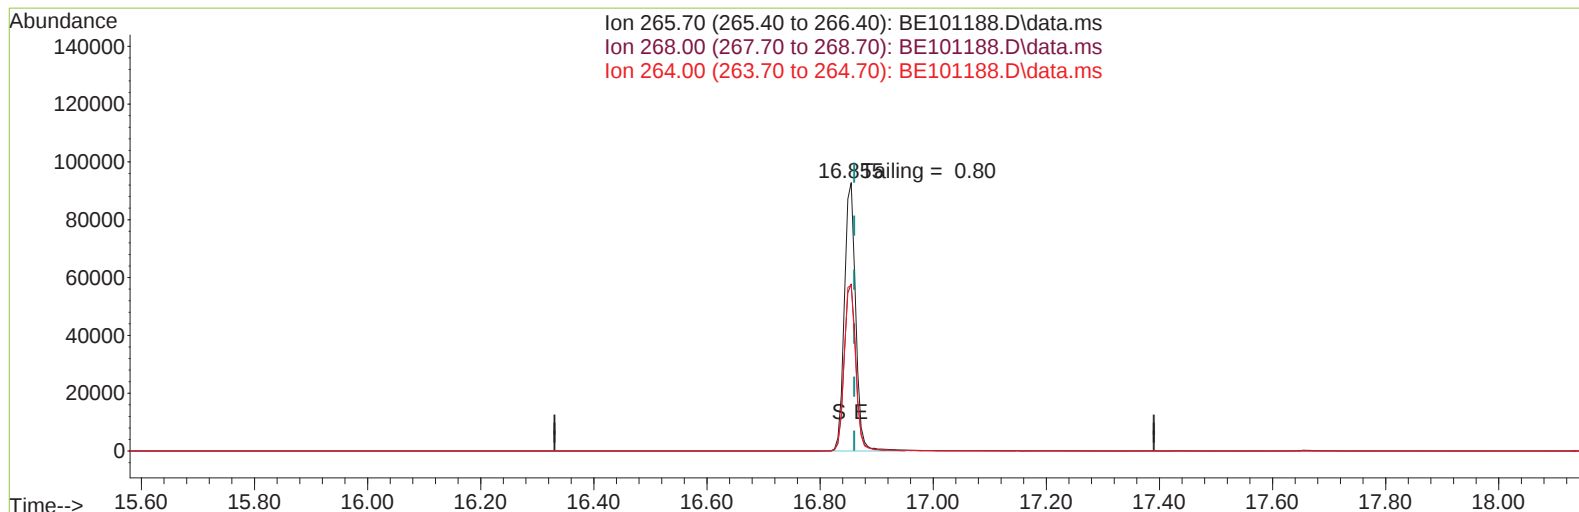

TIC: BE101188.D\data.ms

(70) Pentachlorophenol (C)




16.855min (-0.005) 433064.22 ng

response 129146

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.22
264.00	61.60	61.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040221\
 Data File : BE101188.D
 Acq On : 2 Apr 2021 7:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 09:26:35 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 31 10:54:22 2021
 Response via : Initial Calibration

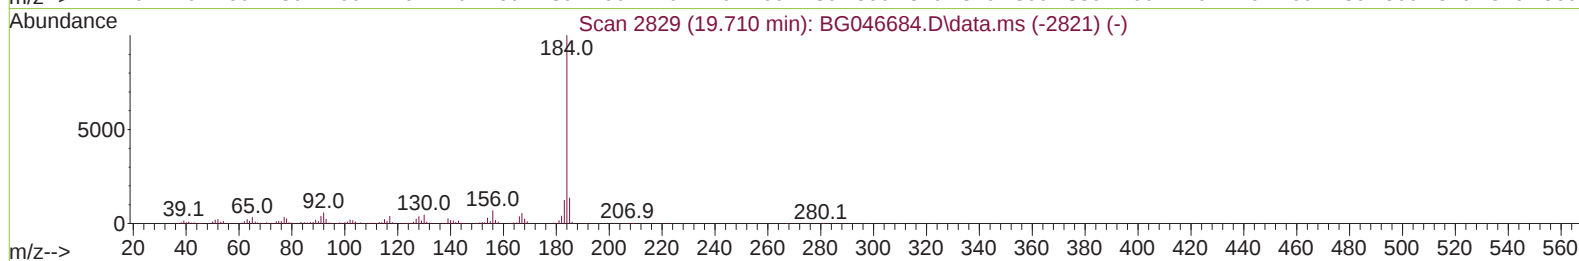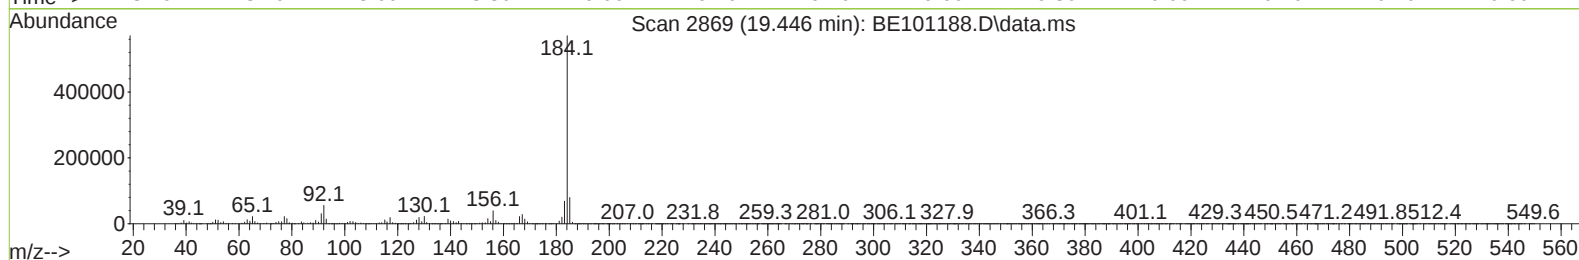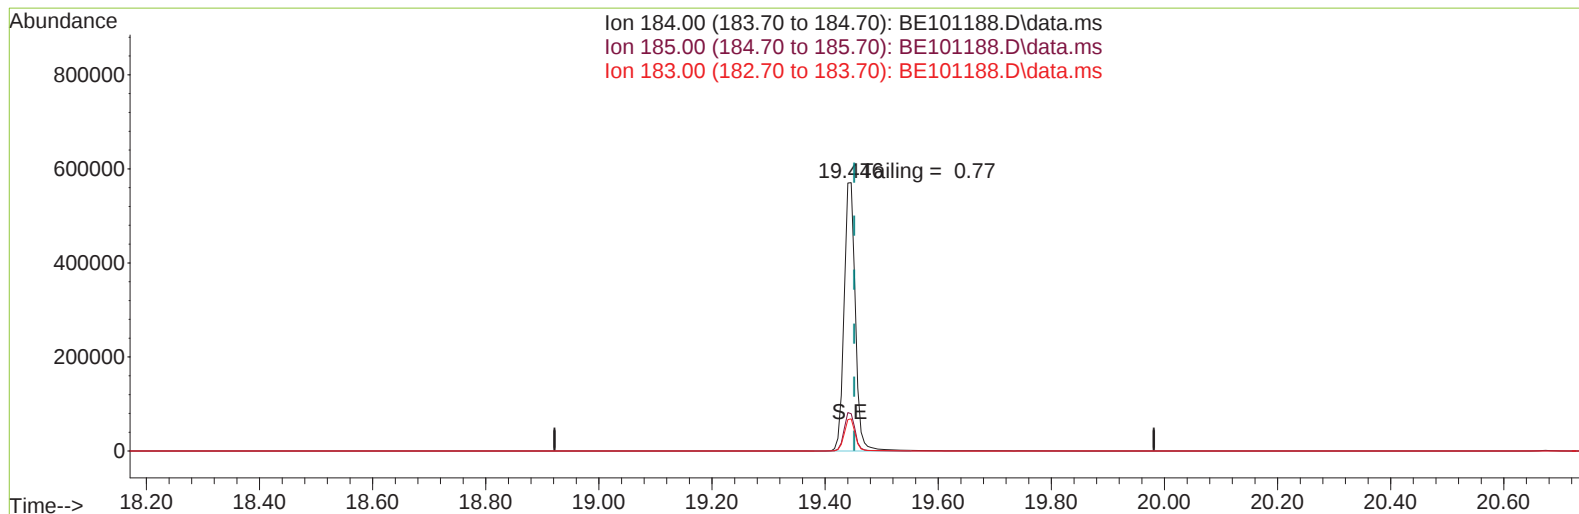

TIC: BE101188.D\data.ms

(77) Benzidine**19.446min (-0.005) 4607.87 ng****response 791869**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.94
183.00	13.20	11.98
0.00	0.00	0.00