
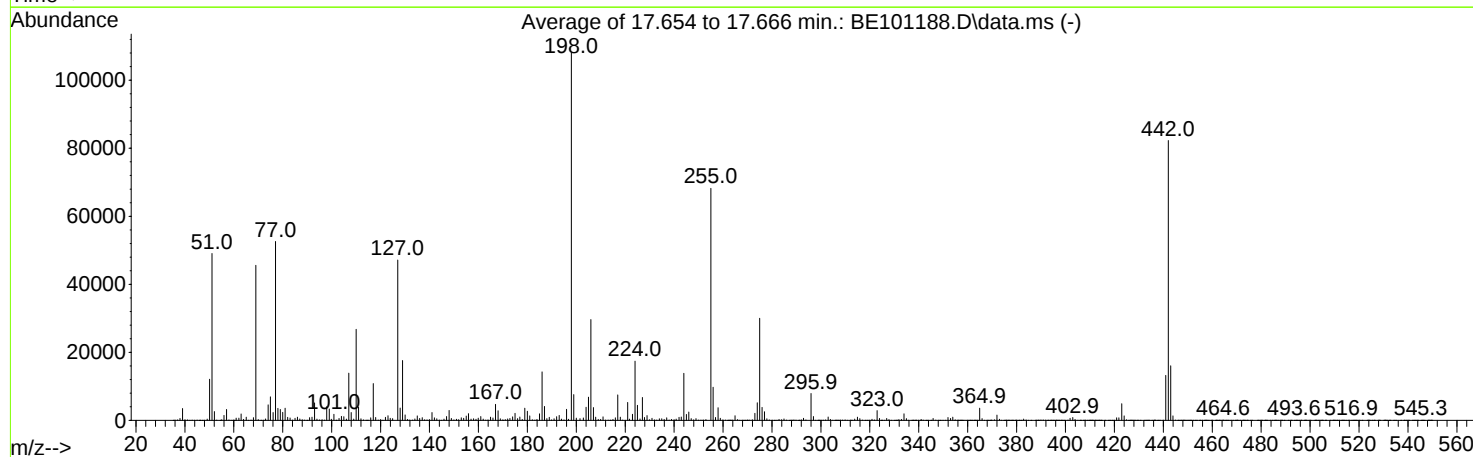


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040221\
 Data File : BE101188.D
 Acq On : 2 Apr 2021 7:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE032421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 02 10:03:59 2021

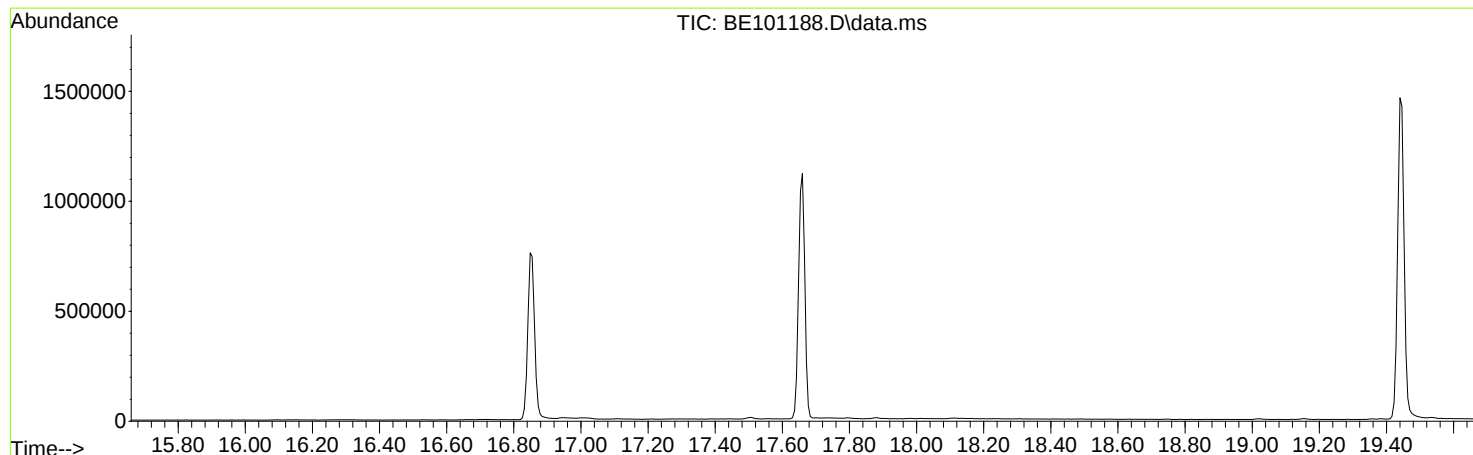

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	49051	PASS
68	69	0.00	2	1.8	812	PASS
69	198	0.00	100	42.2	45593	PASS
70	69	0.00	2	0.6	263	PASS
127	198	10	80	43.6	47158	PASS
197	198	0.00	2	0.3	333	PASS
198	198	100	100	100.0	108154	PASS
199	198	5	9	7.0	7568	PASS
275	198	10	60	27.8	30036	PASS
365	198	1	100	3.3	3557	PASS
441	198	0.01	100	12.2	13222	PASS
442	442	50	100	100.0	82295	PASS
443	442	15	24	19.5	16066	PASS

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/2/2021	BNA_E	<u>BE101188.D</u>
Compound Name	Response	Retention Time
DDT	382181	20.674
DDD	3365	20.239
DDE	723	19.734
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4088	386269	1.06

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040221\
 Data File : BE101188.D
 Acq On : 2 Apr 2021 7:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Quant Time: Apr 02 09:26:35 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 31 10:54:22 2021
 Response via : Initial Calibration

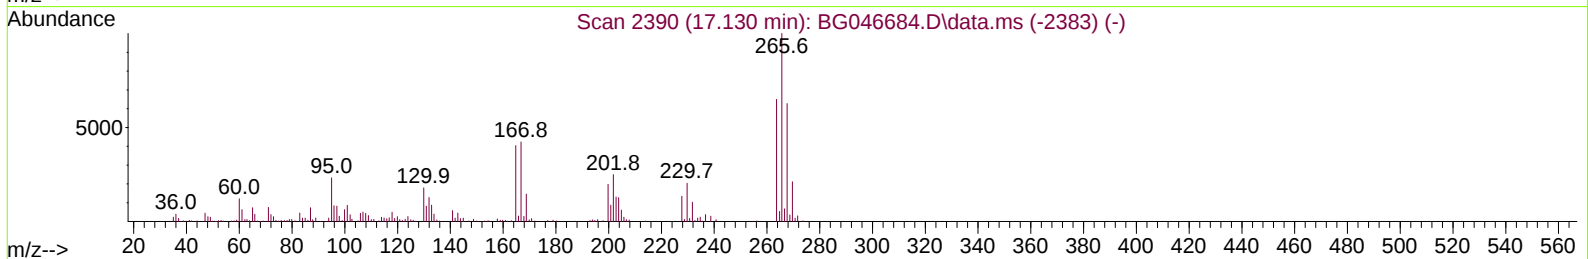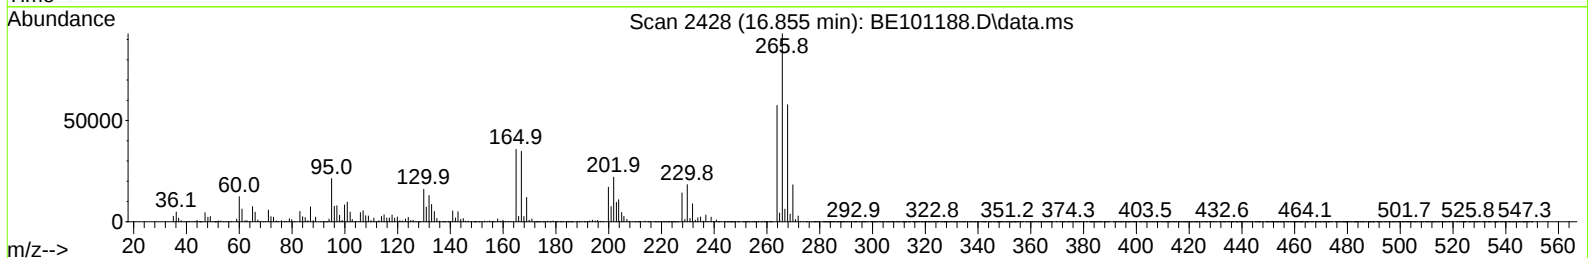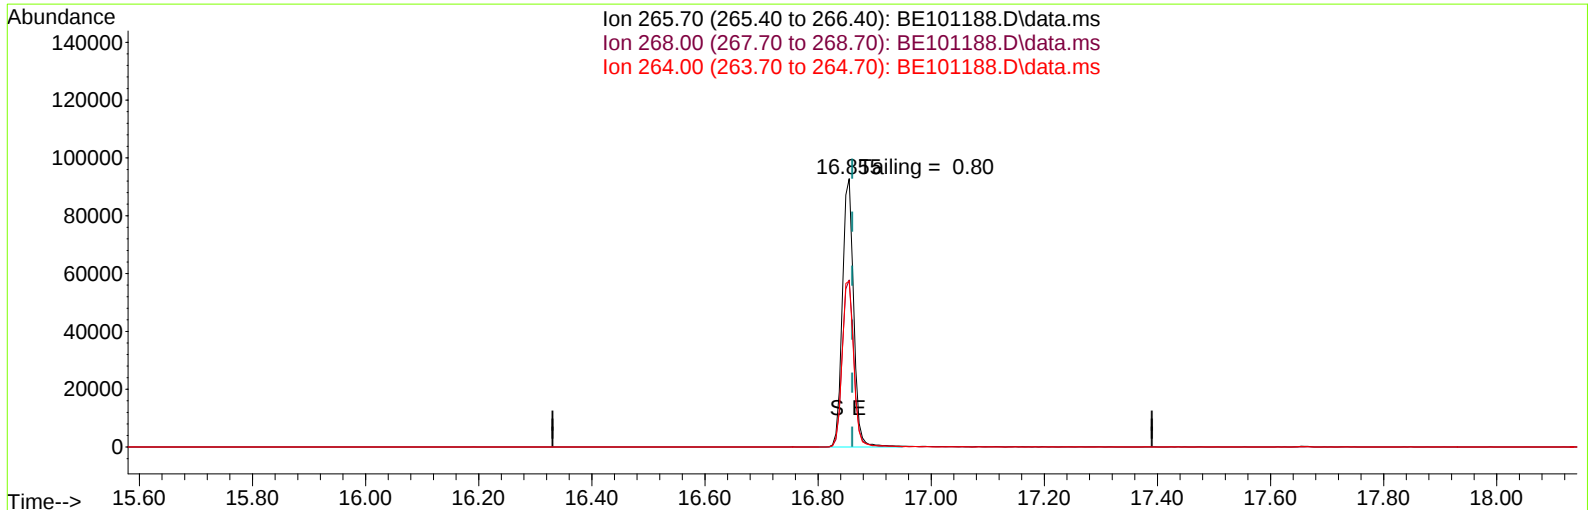

TIC: BE101188.D\data.ms

(70) Pentachlorophenol (C)

16.855min (-0.005) 433064.22 ng




response 129146

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.22
264.00	61.60	61.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040221\
Data File : BE101188.D
Acq On : 2 Apr 2021 7:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Apr 02 09:26:35 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 10:54:22 2021
Response via : Initial Calibration

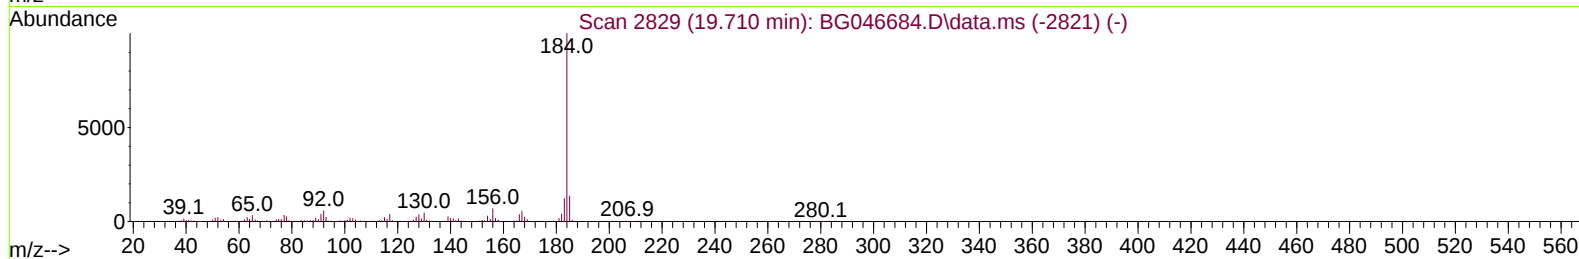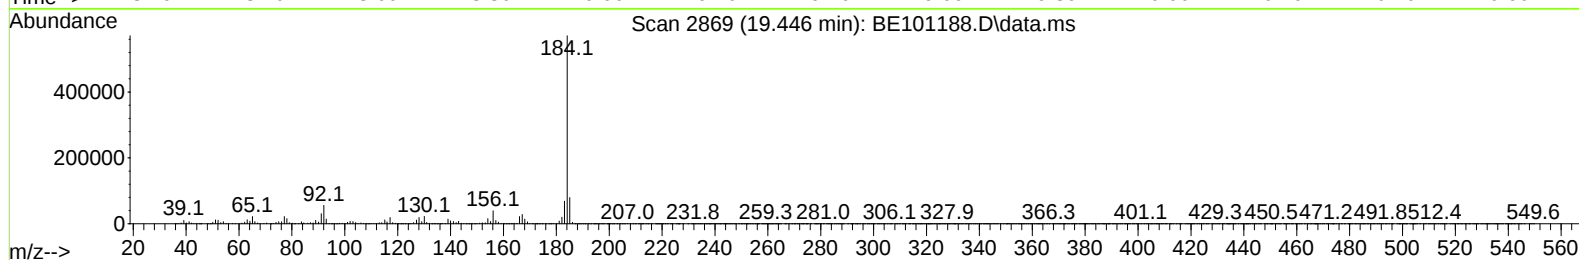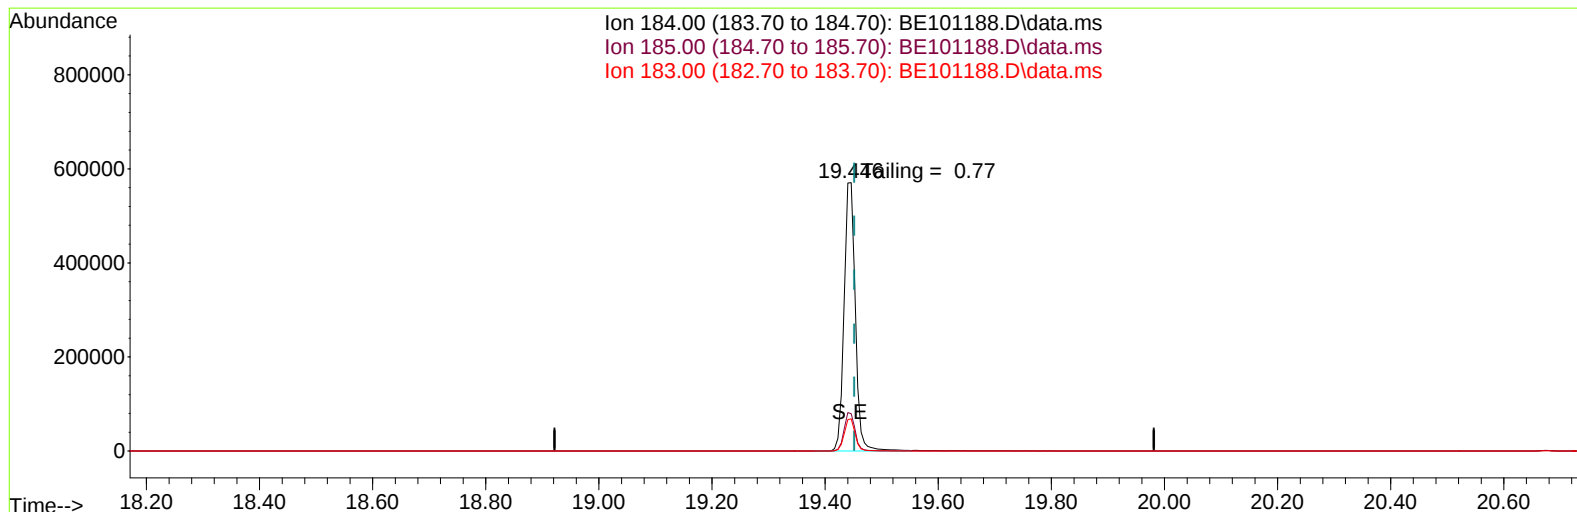

TIC: BE101188.D\data.ms

(77) Benzidine

19.446min (-0.005) 4607.87 ng

response 791869

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.94
183.00	13.20	11.98
0.00	0.00	0.00