

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE040519\
 Data File : BE099306.D
 Acq On : 5 Apr 2019 13:29
 Operator : JU/SJ
 Sample : K2247-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 OUTFALL001-190402

Quant Time: Apr 05 15:01:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE040219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 05 14:55:44 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	3069	0.40	ng	0.00
7) Naphthalene-d8	10.60	136	10922	0.40	ng	-0.01
13) Acenaphthene-d10	14.46	164	7136	0.40	ng	0.00
19) Phenanthrene-d10	17.19	188	21847	0.40	ng	0.00
27) Chrysene-d12	21.37	240	33848	0.40	ng	0.00
34) Perylene-d12	23.86	264	34900	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.39	112	1293	0.16	ng	0.00
5) Phenol-d6	6.98	99	1664	0.15	ng	0.00
8) Nitrobenzene-d5	8.96	82	3100	0.41	ng	0.00
11) 2-Methylnaphthalene-d10	12.19	152	7814	0.41	ng	0.00
14) 2,4,6-Tribromophenol	15.94	330	1226	0.37	ng	0.00
15) 2-Fluorobiphenyl	13.09	172	12276	0.44	ng	0.00
25) Fluoranthene-d10	19.22	212	131970	0.46	ng	0.00
29) Terphenyl-d14	19.81	244	26746	0.43	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.32	88	115	0.028	ng	Qvalue # 1
32) Bis(2-ethylhexyl)phthalate	21.27	149	16868	0.124	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE040519\
Data File : BE099306.D
Acq On : 5 Apr 2019 13:29
Operator : JU/SJ
Sample : K2247-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
OUTFALL001-190402

Quant Time: Apr 05 15:01:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE040219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 05 14:55:44 2019
Response via : Initial Calibration

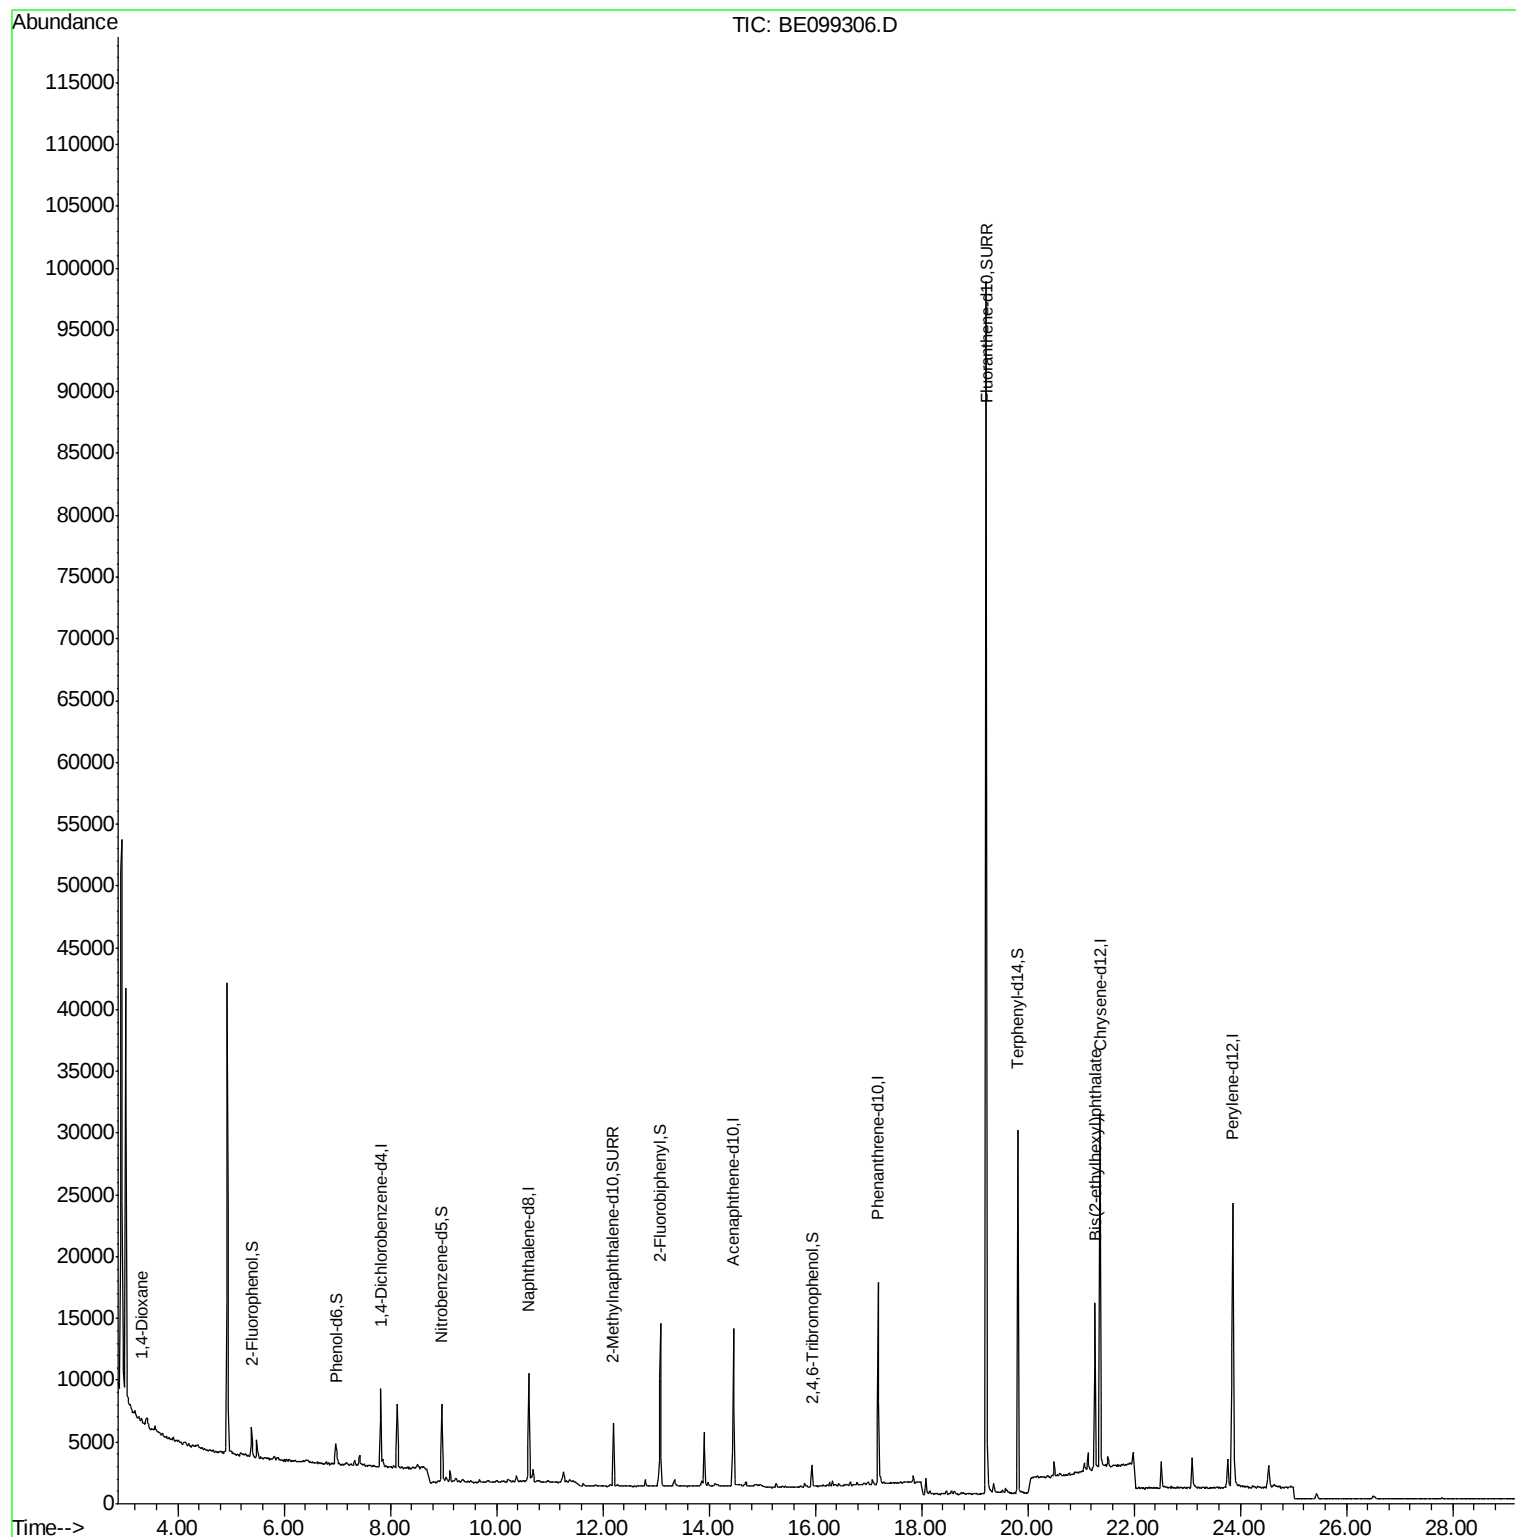

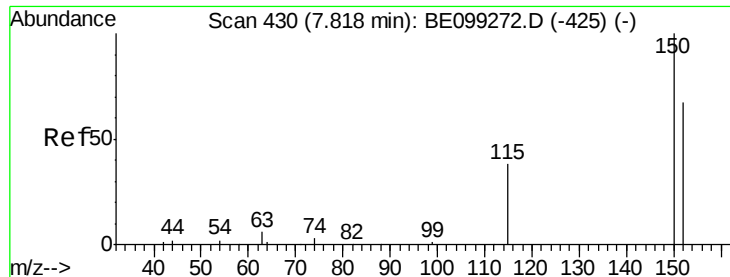


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.82 min Scan# 430
Delta R.T. 0.00 min
Lab File: BE099306.D
Acq: 5 Apr 2019 13:29

Instrument :
BNA_E
ClientSampleId :
OUTFALL001-190402

Tot Ion:152 Resp: 3069
Ion Ratio Lower Upper
152 100
150 144.5 120.2 180.2
115 59.0 50.2 75.2

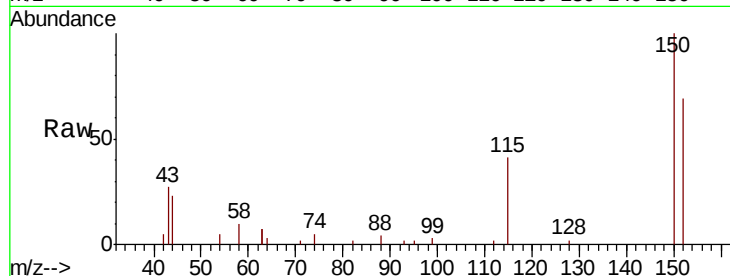


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

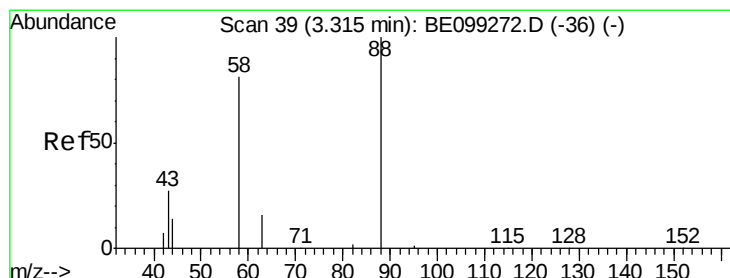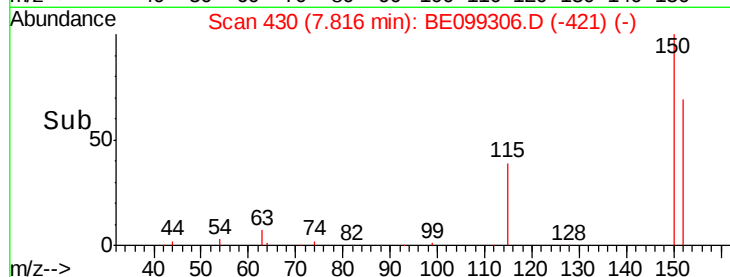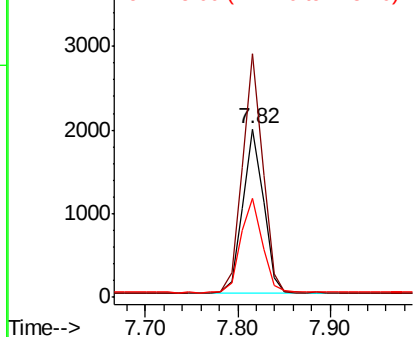



#2


1,4-Dioxane
Concen: 0.028 ng
RT: 3.32 min Scan# 40
Delta R.T. 0.00 min
Lab File: BE099306.D
Acq: 5 Apr 2019 13:29

Tgt Ion: 88 Resp: 115
Ion Ratio Lower Upper
88 100
58 0.0 43.8 65.8#
43 680.0 18.6 28.0#

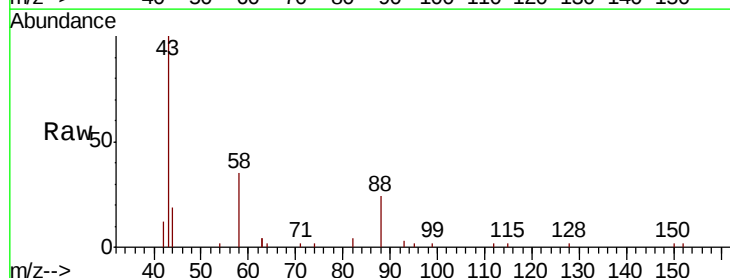

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

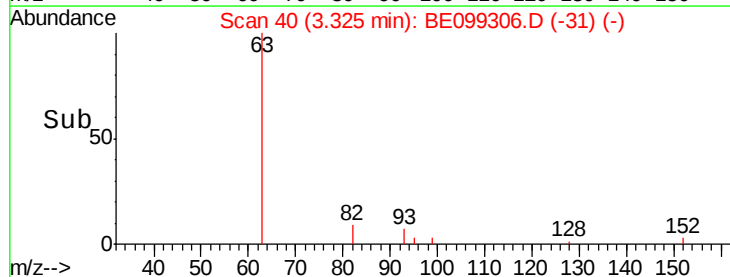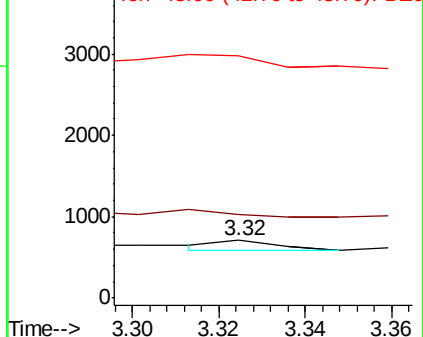

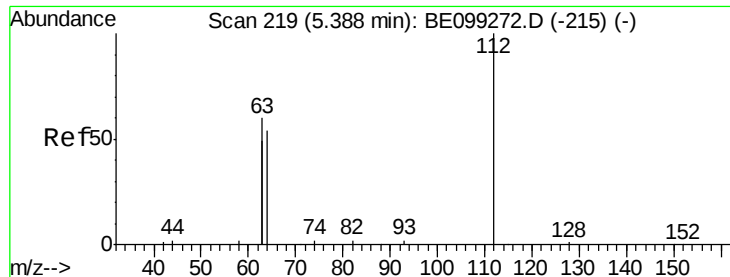

#4

2-Fluorophenol

Concen: 0.159 ng

RT: 5.39 min Scan# 219

Delta R.T. 0.00 min

Lab File: BE099306.D

Acq: 5 Apr 2019 13:29

Instrument :

BNA_E

ClientSampleId :

OUTFALL001-190402


Tot Ion:112 Resp: 1293

Ion Ratio Lower Upper

112 100

64 57.7 44.8 67.2




63 115.2 94.8 142.2

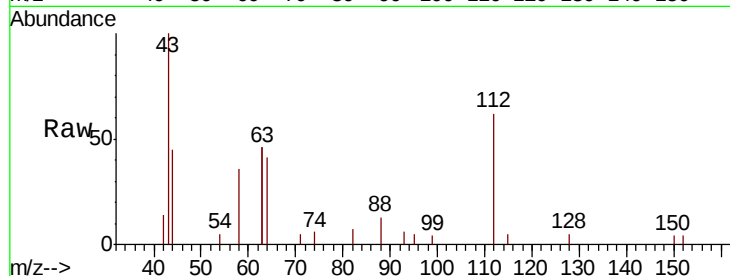

Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

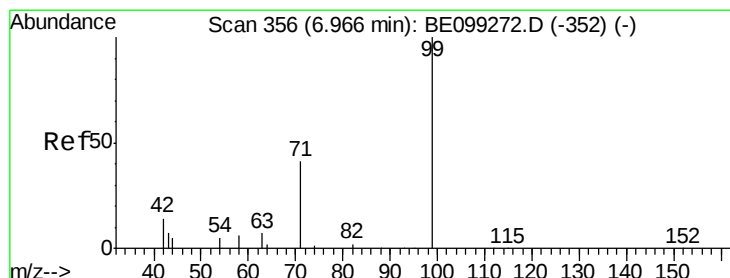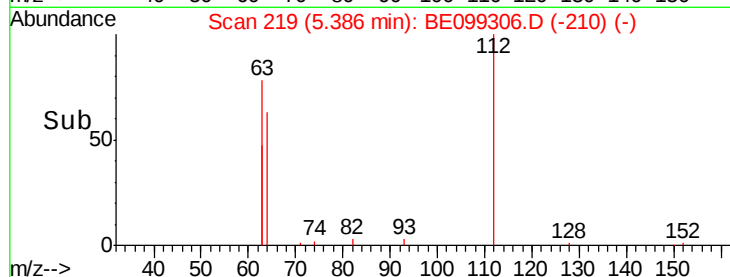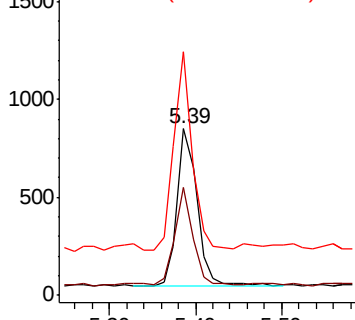

#5

Phenol-d6

Concen: 0.148 ng

RT: 6.98 min Scan# 357

Delta R.T. 0.00 min

Lab File: BE099306.D

Acq: 5 Apr 2019 13:29


Tgt Ion: 99 Resp: 1664

Ion Ratio Lower Upper

99 100

42 14.8 12.4 18.6



71 41.0 30.0 45.0

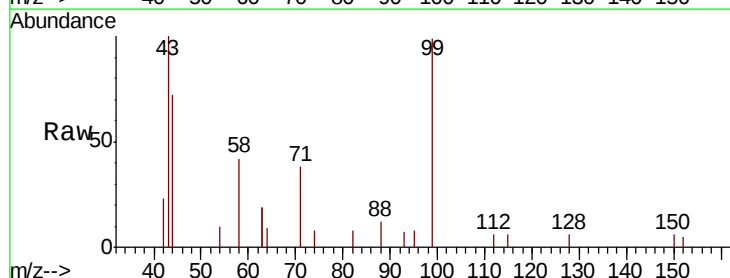


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

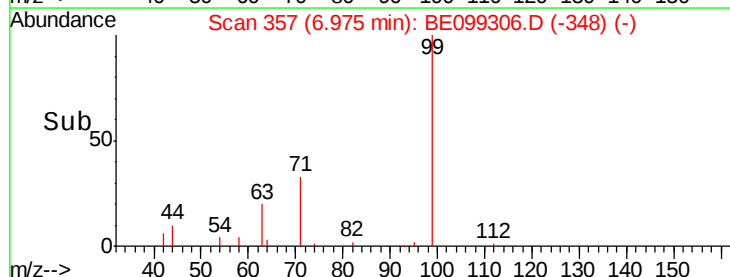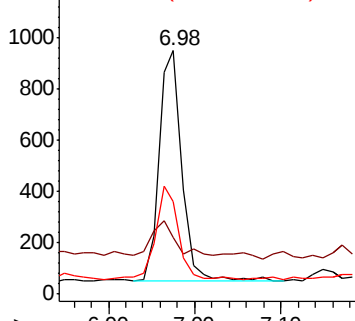

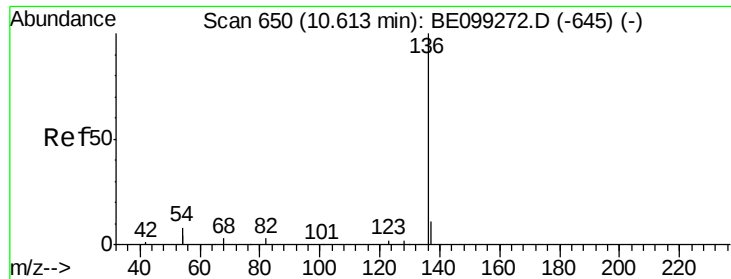

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.60 min Scan# 649

Delta R.T. -0.01 min

Lab File: BE099306.D

Acq: 5 Apr 2019 13:29

Instrument :

BNA_E

ClientSampleId :

OUTFALL001-190402

Tot Ion:136 Resp: 10922


Ion Ratio Lower Upper

136 100

137 12.1 8.3 12.5

54 34.3 10.8 16.2#

68 8.6 3.2 4.8#

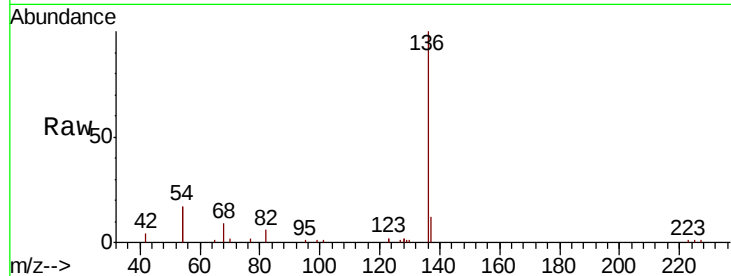


Abundance Ion 136.00 (135.70 to 136.70): E



Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0



Time-->

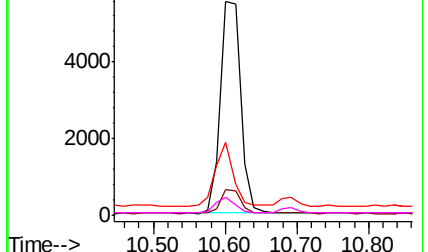

#8

Nitrobenzene-d5

Concen: 0.413 ng

RT: 8.96 min Scan# 523

Delta R.T. -0.00 min

Lab File: BE099306.D

Acq: 5 Apr 2019 13:29


Tgt Ion: 82 Resp: 3100

Ion Ratio Lower Upper

82 100

128 117.0 90.1 135.1


54 169.0 123.6 185.4




Abundance Ion 82.00 (81.70 to 82.70): BE0


Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0



Time-->




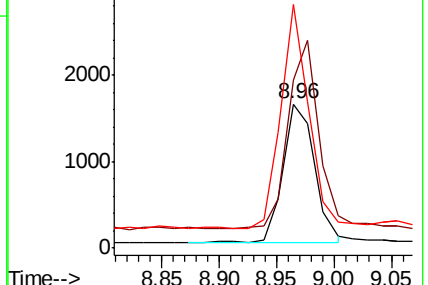




#11
 2-Methylnaphthalene-d10
 Concen: 0.410 ng
 RT: 12.19 min Scan# 762
 Delta R.T. -0.00 min
 Lab File: BE099306.D
 Acq: 5 Apr 2019 13:29




Instrument :
 BNA_E
 ClientSampleId :
 OUTFALL001-190402


Tot Ion:152 Resp: 7814
 Ion Ratio Lower Upper
 152 100
 151 19.7 15.1 22.7

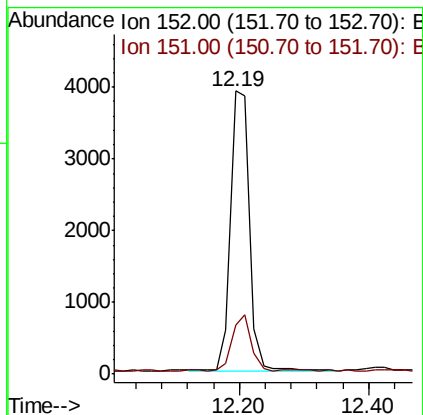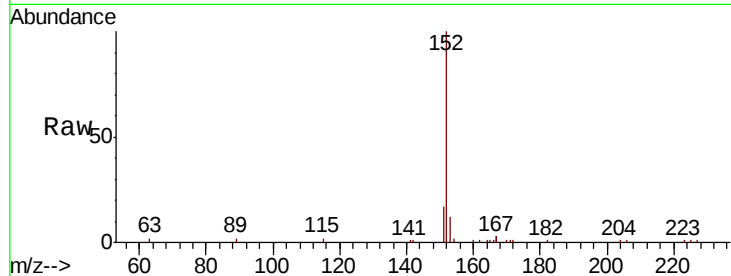

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.46 min Scan# 919
 Delta R.T. -0.00 min
 Lab File: BE099306.D
 Acq: 5 Apr 2019 13:29

Tgt Ion:164 Resp: 7136
 Ion Ratio Lower Upper
 164 100
 162 96.9 78.7 118.1
 160 46.5 37.8 56.8

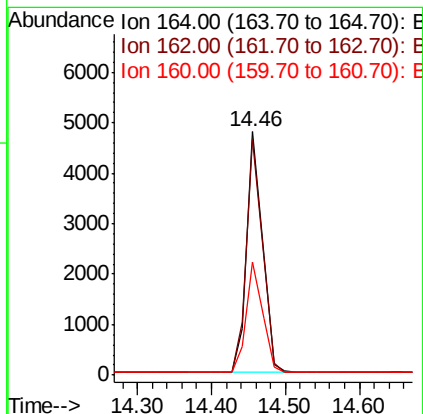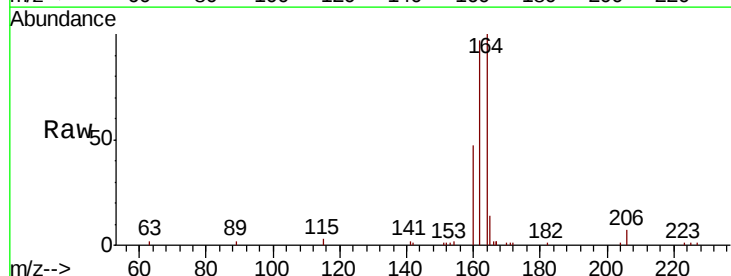



#14

2,4,6-Tribromophenol

Concen: 0.373 ng

RT: 15.94 min Scan# 1024

Delta R.T. 0.00 min

Lab File: BE099306.D

Acq: 5 Apr 2019 13:29

Instrument :

BNA_E

ClientSampleId :

OUTFALL001-190402


Tot Ion:330 Resp: 1226

Ion Ratio Lower Upper

330 100

332 96.2 82.0 123.0




141 30.5 25.4 38.2

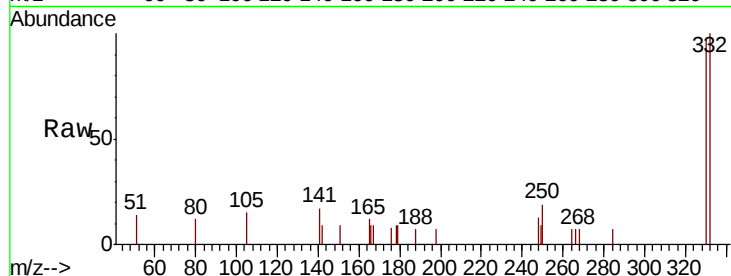

Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

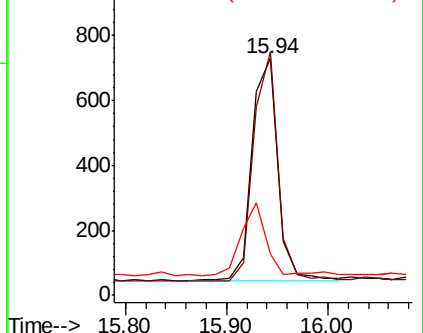

#15

2-Fluorobiphenyl

Concen: 0.438 ng

RT: 13.09 min Scan# 824

Delta R.T. -0.00 min

Lab File: BE099306.D

Acq: 5 Apr 2019 13:29


Tgt Ion:172 Resp: 12276

Ion Ratio Lower Upper

172 100

171 34.3 27.0 40.4



170 24.0 17.8 26.6




Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

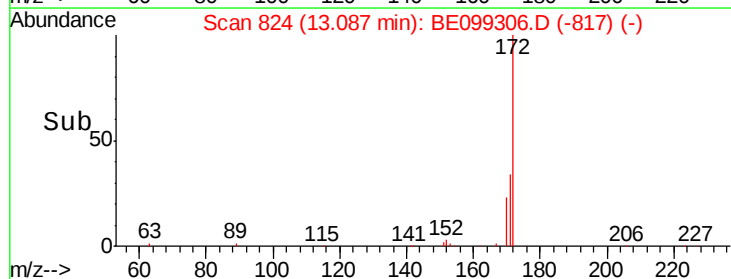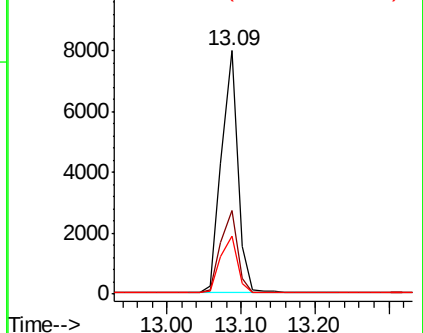

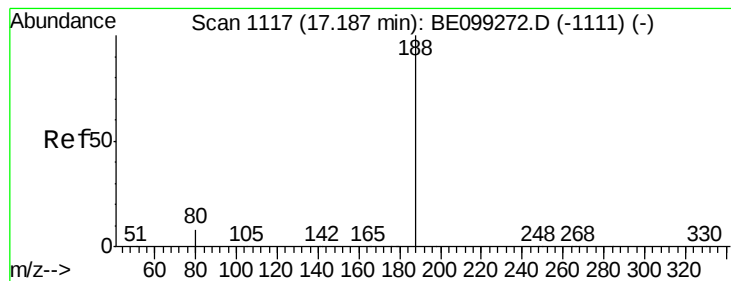

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.19 min Scan# 1117

Delta R.T. 0.00 min

Lab File: BE099306.D

Acq: 5 Apr 2019 13:29

Instrument :

BNA_E

ClientSampleId :

OUTFALL001-190402


Tot Ion:188 Resp: 21847

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 7.4 7.5 11.3#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

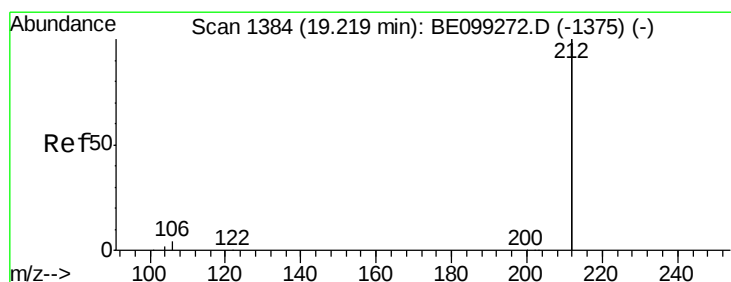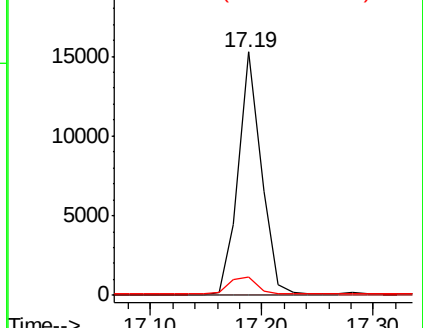

#25

Fluoranthene-d10

Concen: 0.458 ng

RT: 19.22 min Scan# 1384

Delta R.T. 0.00 min

Lab File: BE099306.D

Acq: 5 Apr 2019 13:29


Tgt Ion:212 Resp: 131970

Ion Ratio Lower Upper

212 100

106 2.2 1.7 2.5



104 1.3 1.0 1.4




Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

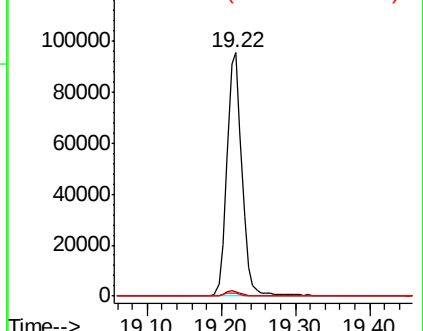



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.37 min Scan# 1630

Delta R.T. 0.00 min

Lab File: BE099306.D

Acq: 5 Apr 2019 13:29

Instrument :

BNA_E

ClientSampleId :

OUTFALL001-190402


Tot Ion:240 Resp: 33848

Ion Ratio Lower Upper

240 100

120 3.1 2.3 3.5

236 25.7 21.0 31.6






Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

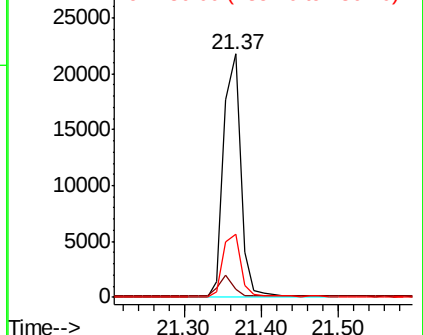

#29

Terphenyl-d14

Concen: 0.433 ng

RT: 19.81 min Scan# 1487

Delta R.T. -0.01 min

Lab File: BE099306.D

Acq: 5 Apr 2019 13:29


Tgt Ion:244 Resp: 26746

Ion Ratio Lower Upper

244 100

212 30.7 22.4 33.6

122 7.7 4.4 6.6#






Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

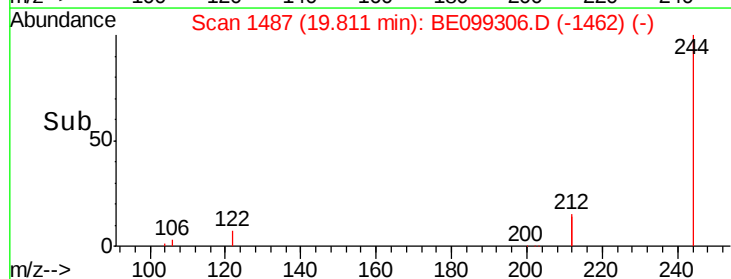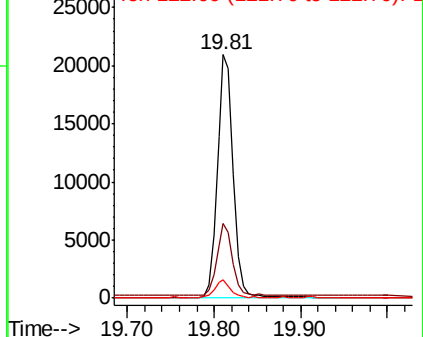



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.124 ng

RT: 21.27 min Scan# 1622

Delta R.T. 0.00 min

Lab File: BE099306.D

Acq: 5 Apr 2019 13:29

Instrument :

BNA_E

ClientSampleId :

OUTFALL001-190402


Tot Ion:149 Resp: 16868

Ion Ratio Lower Upper

149 100

167 7.3 5.8 8.6




279 1.3 1.0 1.6



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

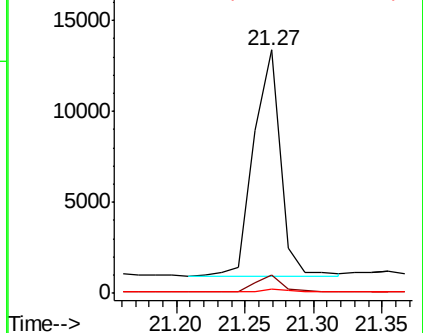

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.86 min Scan# 2197

Delta R.T. -0.00 min

Lab File: BE099306.D

Acq: 5 Apr 2019 13:29


Tgt Ion:264 Resp: 34900

Ion Ratio Lower Upper

264 100

260 24.5 19.9 29.9

265 26.0 20.3 30.5



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

