


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE040519\
Data File : BE099301.D
Acq On : 5 Apr 2019 9:39
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE040219.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Apr 02 17:16:42 2019

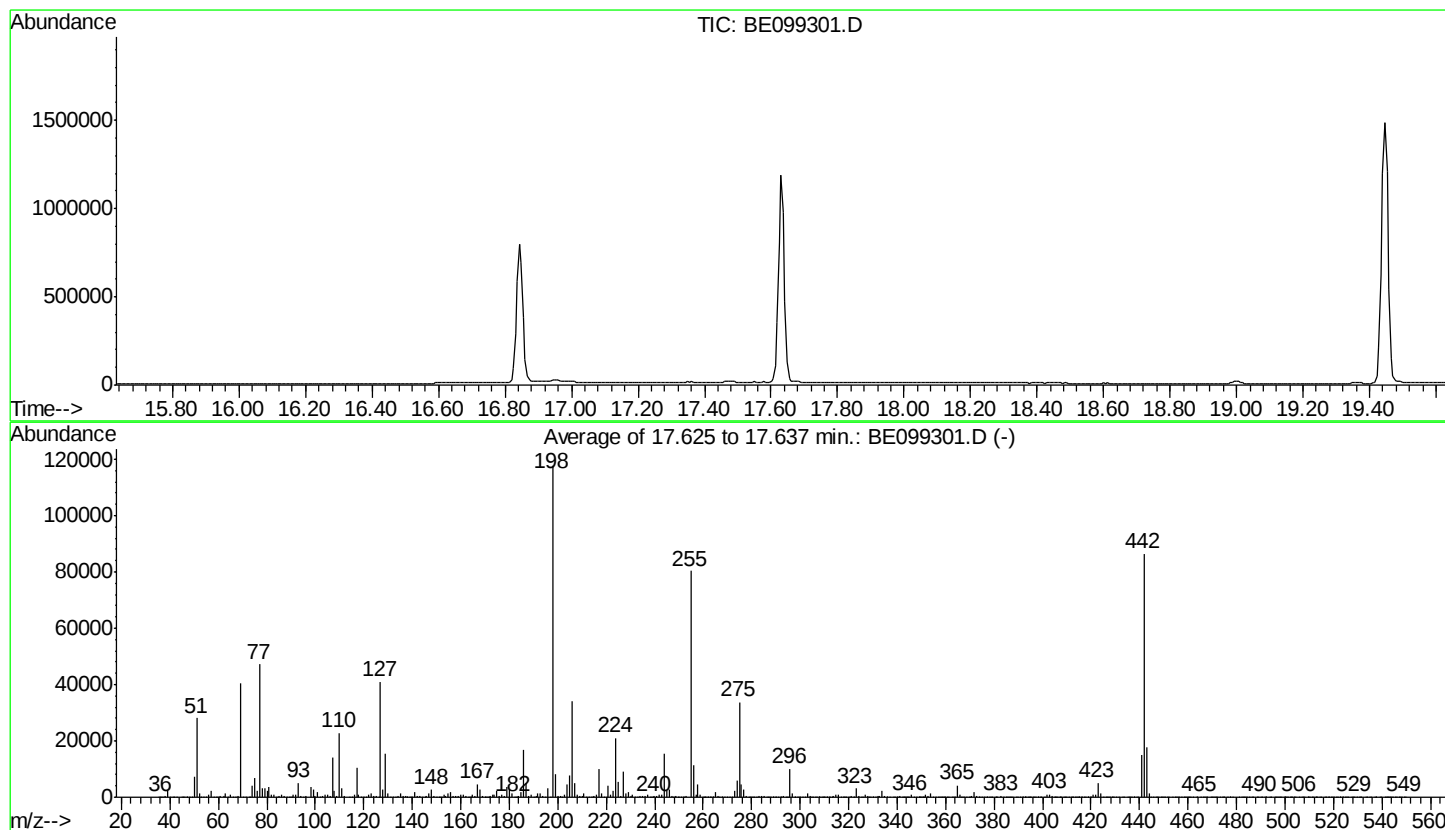

AutoFind: Scans 2559, 2560, 2561; Background Corrected with Scan 2552

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.9	28120	PASS
68	69	0.00	2	1.6	646	PASS
69	198	0.00	100	34.5	40629	PASS
70	69	0.00	2	0.3	113	PASS
127	198	10	80	34.8	40907	PASS
197	198	0.00	2	0.2	224	PASS
198	198	100	100	100.0	117707	PASS
199	198	5	9	6.8	7998	PASS
275	198	10	60	28.6	33720	PASS
365	198	1	100	3.6	4239	PASS
441	198	0.01	100	12.7	14944	PASS
442	198	50	100	73.4	86352	PASS
443	442	15	24	20.5	17693	PASS