
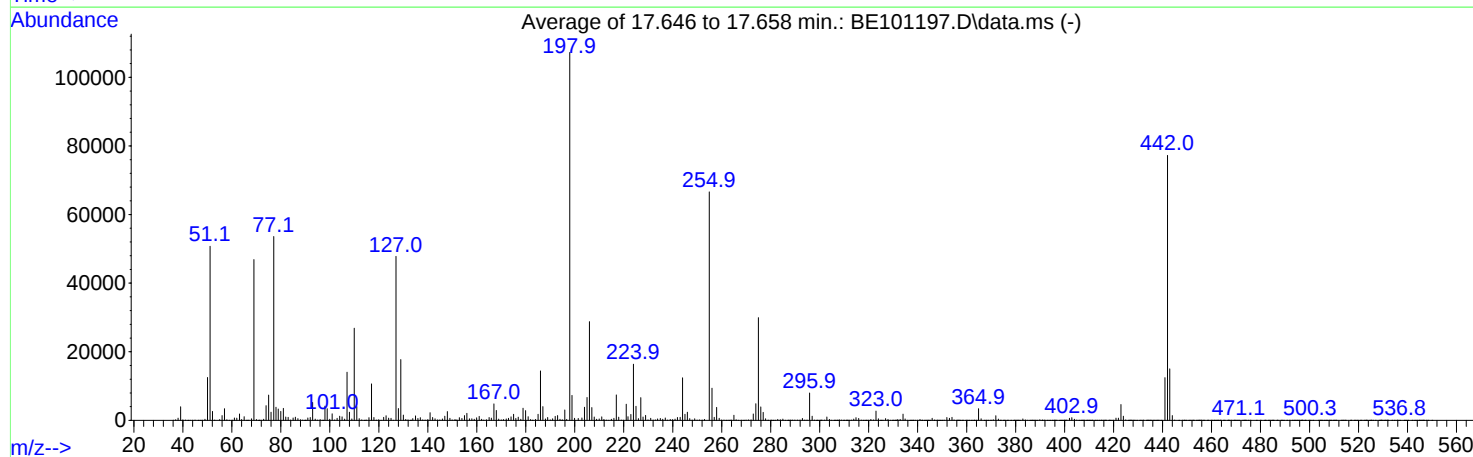


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040521\
 Data File : BE101197.D
 Acq On : 5 Apr 2021 14:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE040521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 06 03:03:09 2021

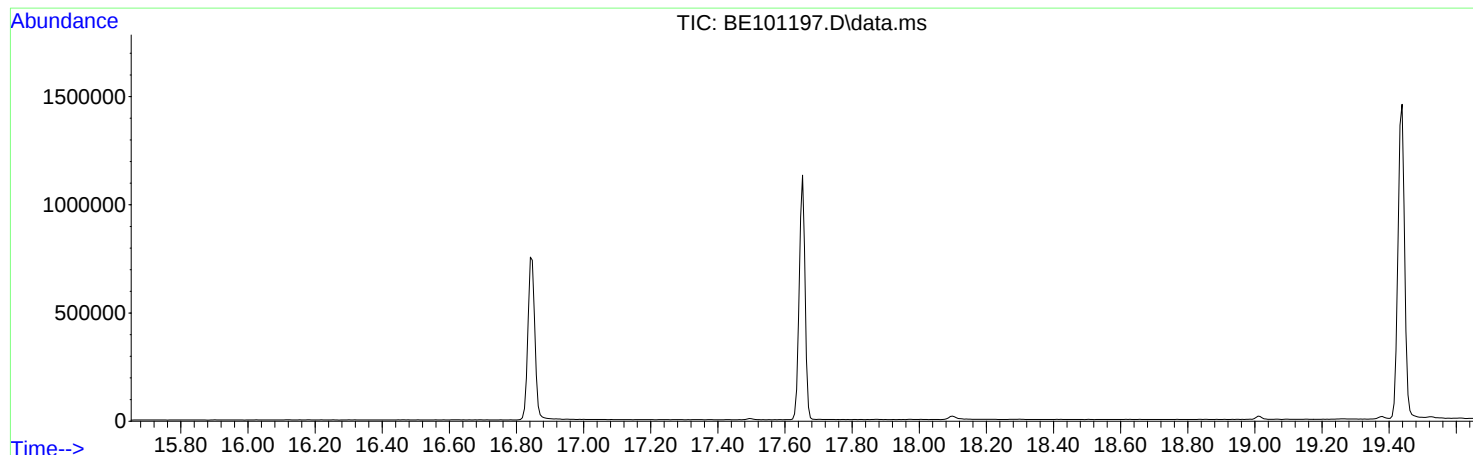




AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.3	50756	PASS
68	69	0.00	2	1.0	465	PASS
69	198	0.00	100	43.7	46879	PASS
70	69	0.00	2	0.5	238	PASS
127	198	10	80	44.6	47795	PASS
197	198	0.00	2	0.3	303	PASS
198	198	100	100	100.0	107241	PASS
199	198	5	9	6.8	7267	PASS
275	198	10	60	27.9	29963	PASS
365	198	1	100	3.2	3404	PASS
441	198	0.01	100	11.6	12440	PASS
442	442	50	100	100.0	77266	PASS
443	442	15	24	19.4	15006	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040521\
Data File : BE101197.D
Acq On : 5 Apr 2021 14:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Apr 05 18:36:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 10:54:22 2021
Response via : Initial Calibration

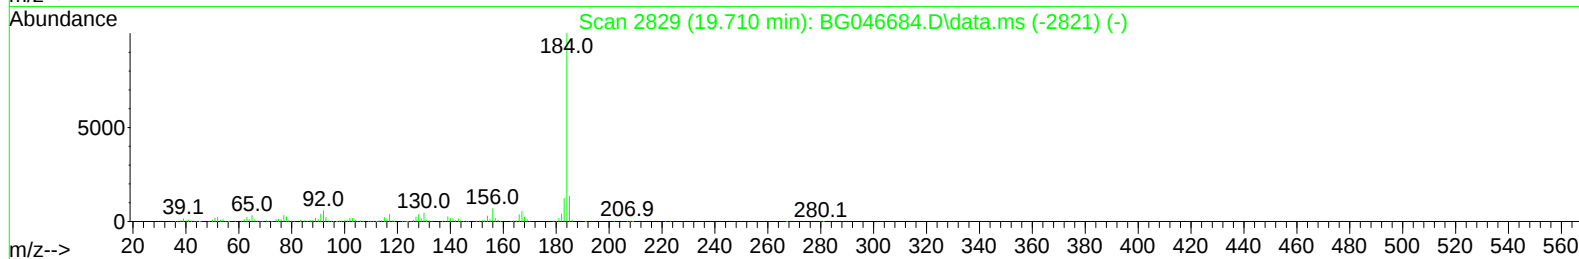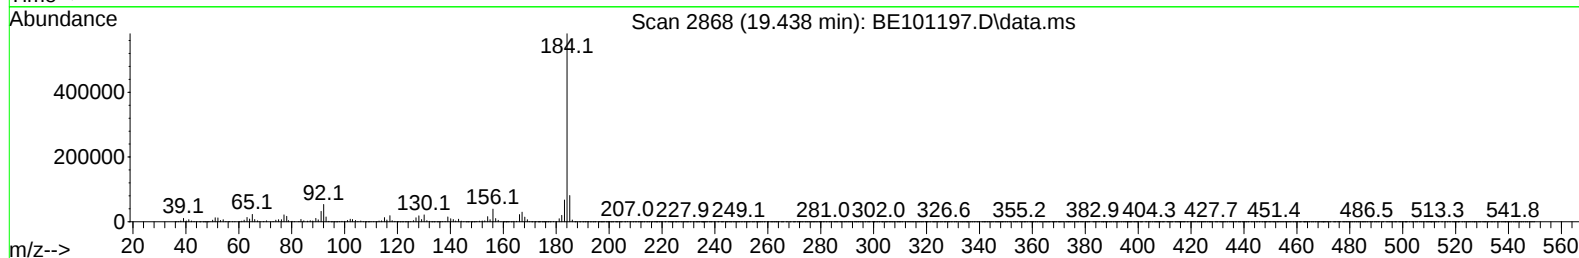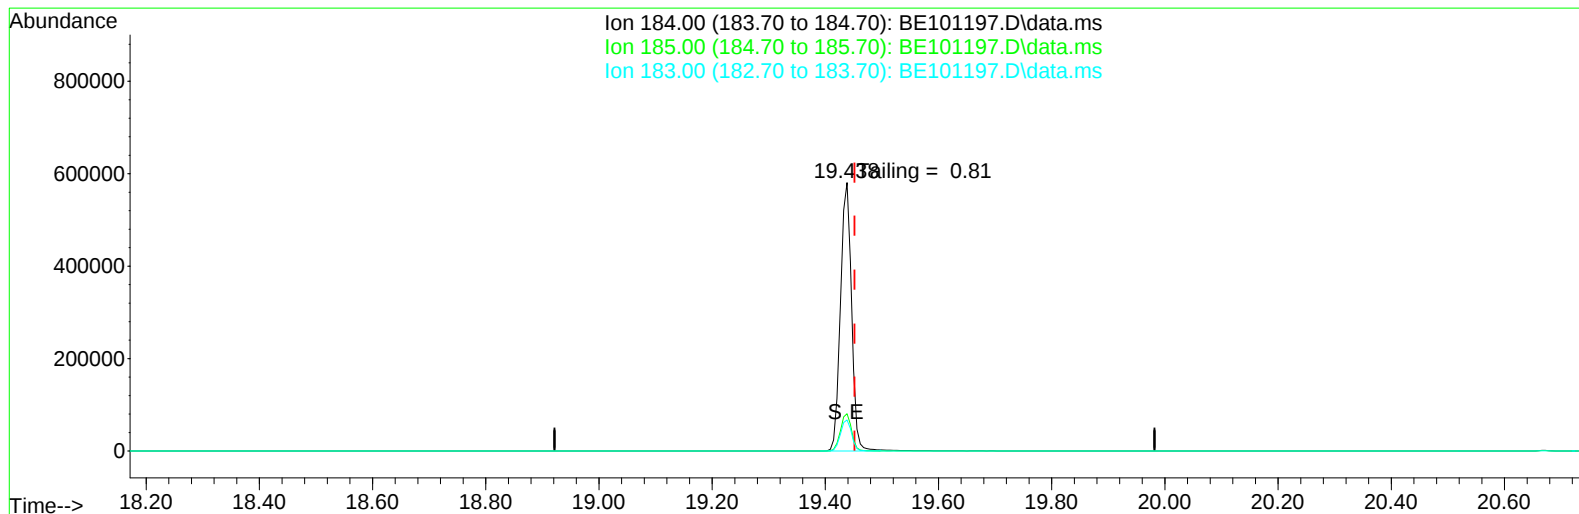

TIC: BE101197.D\data.ms

(77) Benzidine

19.438min (-0.013) 4614.48 ng




response 792152

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.93
183.00	13.20	11.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040521\
 Data File : BE101197.D
 Acq On : 5 Apr 2021 14:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Quant Time: Apr 05 18:36:40 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 31 10:54:22 2021
 Response via : Initial Calibration

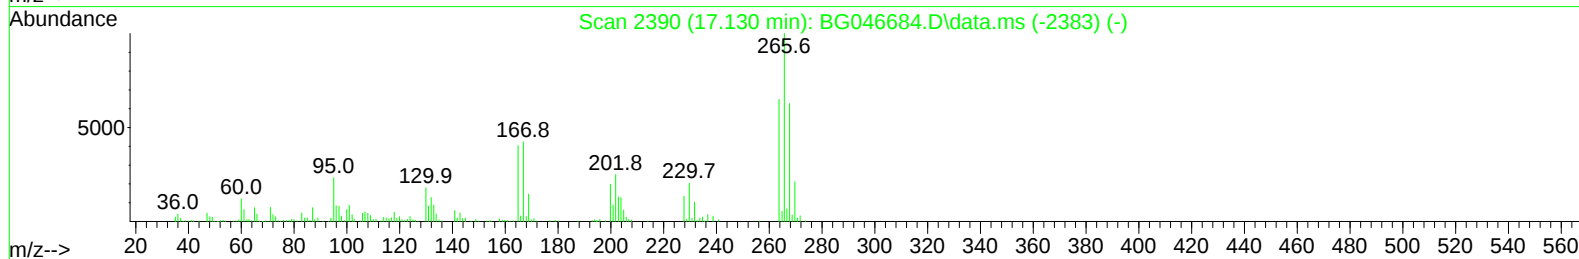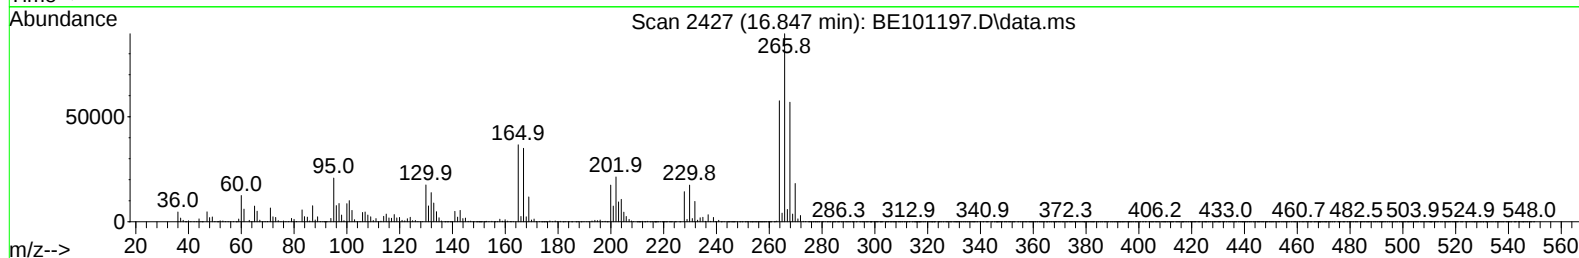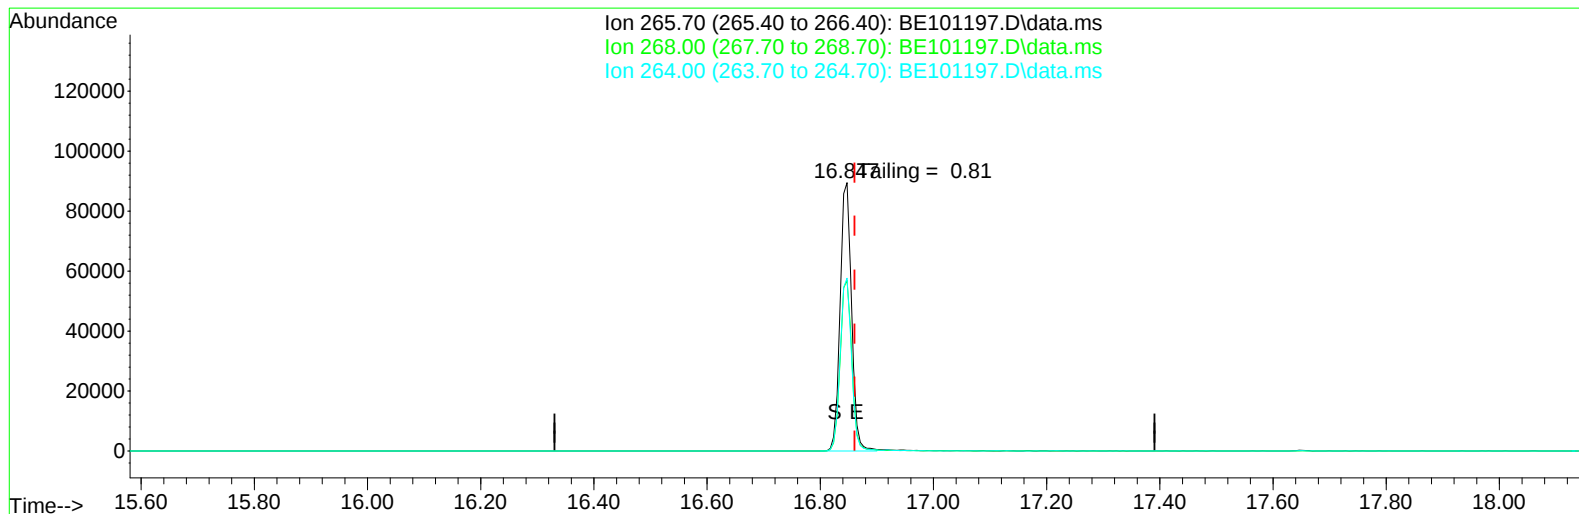

TIC: BE101197.D\data.ms

(70) Pentachlorophenol (C)

16.847min (-0.013) 2676946.22 ng

response 126048

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.57
264.00	61.60	64.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/5/2021	BNA_E	BE101197.D
Compound Name	Response	Retention Time
DDT	393668	20.67
DDD	2748	20.23
DDE	595	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3343	397011	0.84

Instrument :
BNA_E
ClientSampleId :
DFTPP