
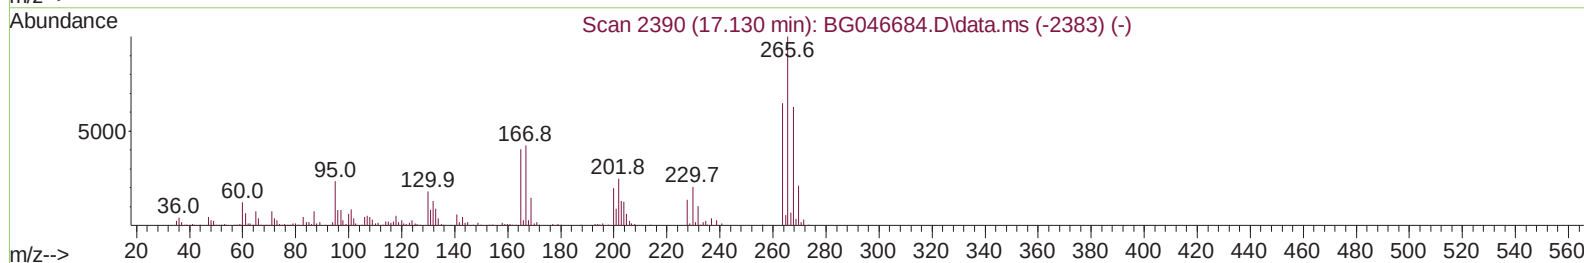
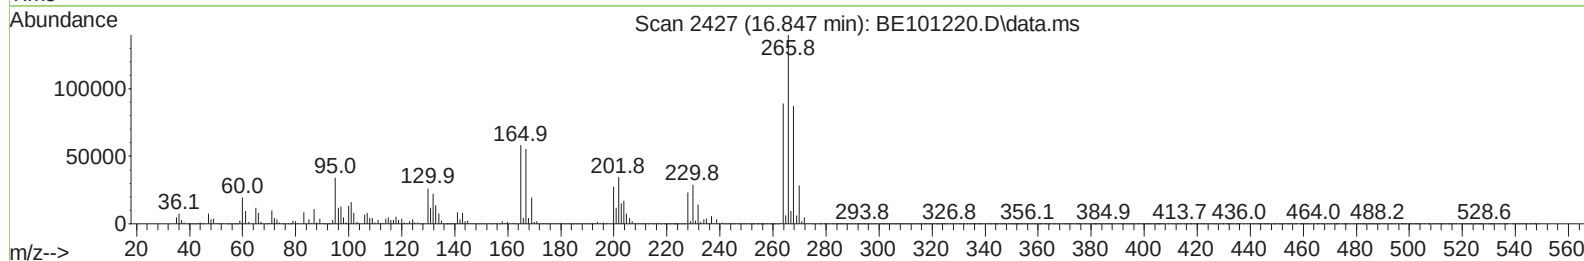


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040721\
Data File : BE101220.D
Acq On : 7 Apr 2021 8:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 10:17:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 10:54:22 2021
Response via : Initial Calibration

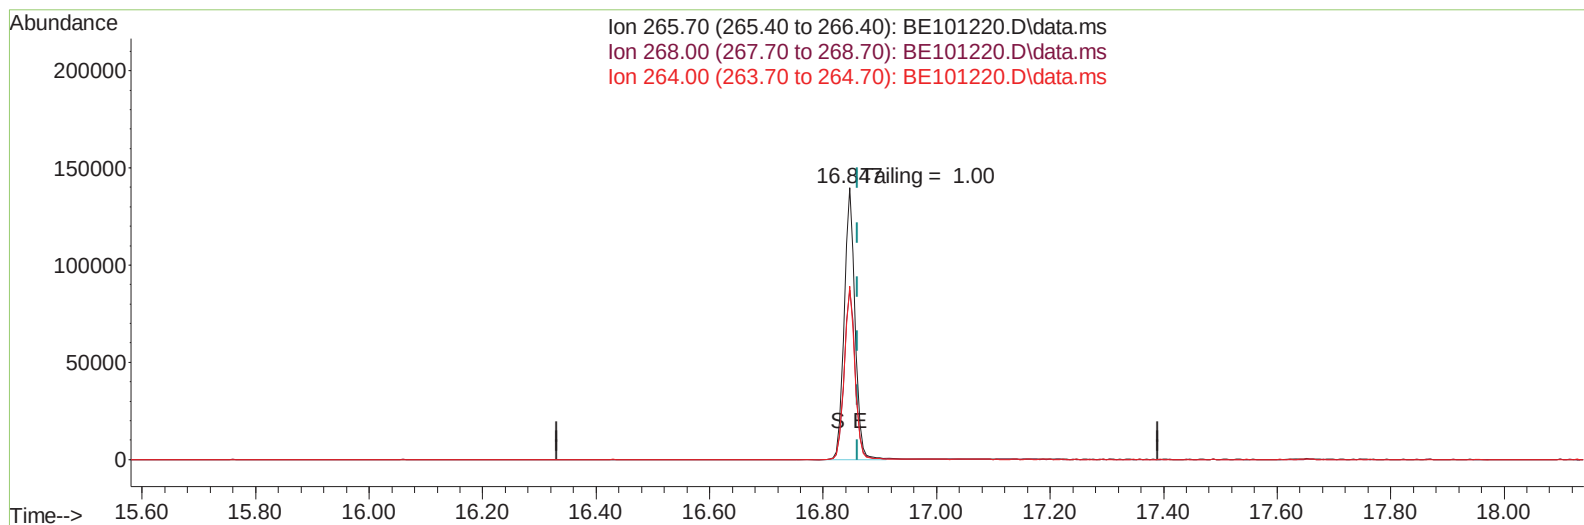




TIC: BE101220.D\data.ms

(70) Pentachlorophenol (C)**16.847min (-0.013) 1698185.03 ng****response 186577**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.40
264.00	61.60	63.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040721\
Data File : BE101220.D
Acq On : 7 Apr 2021 8:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 10:17:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 10:54:22 2021
Response via : Initial Calibration

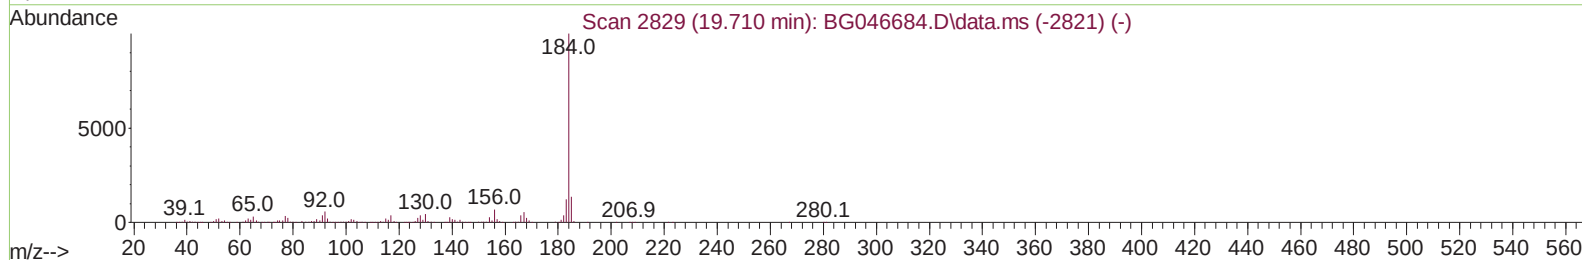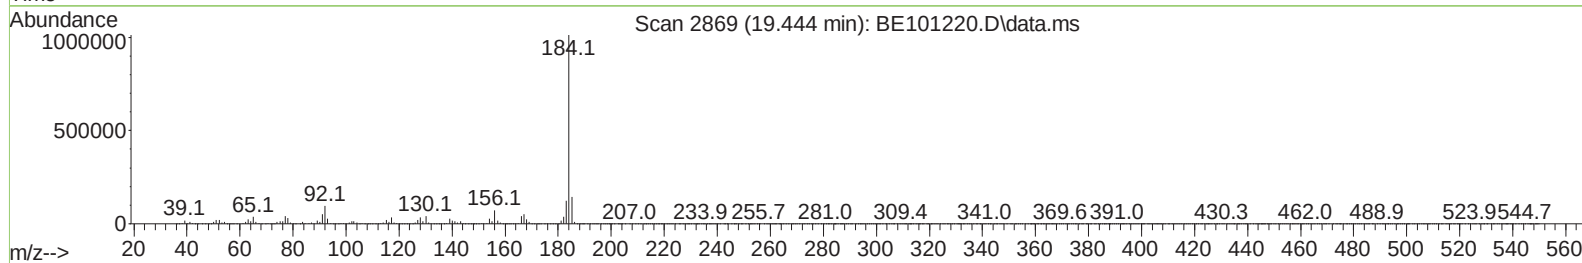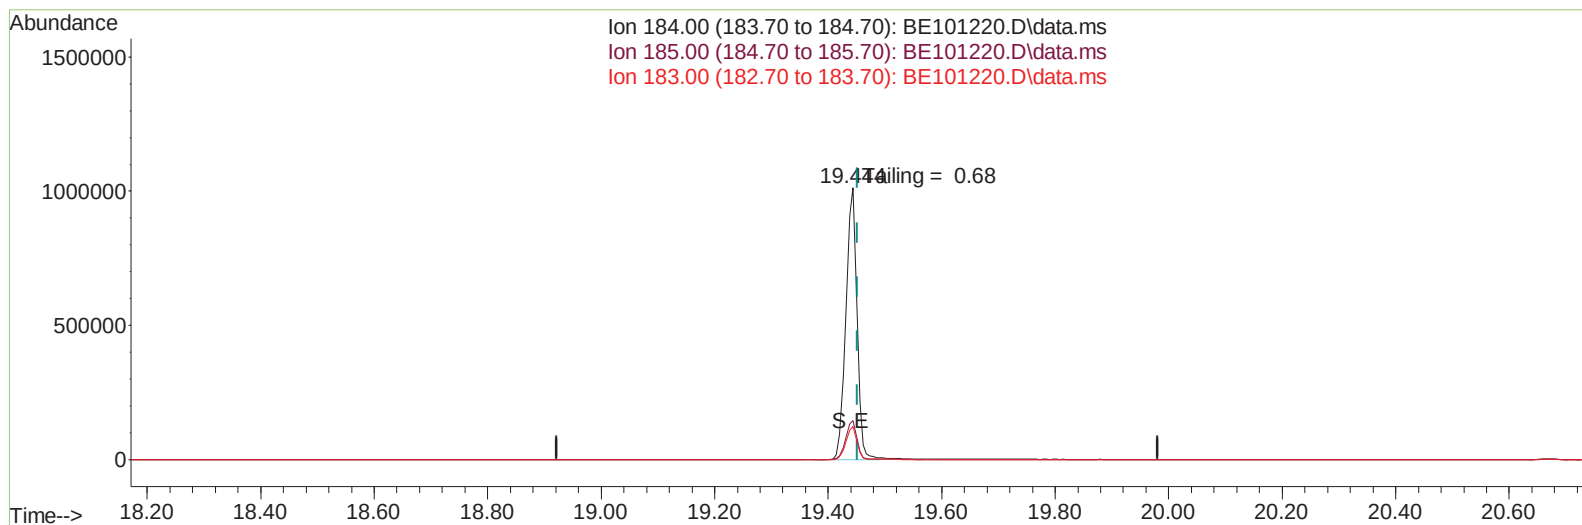

TIC: BE101220.D\data.ms

(77) Benzidine**19.444min (-0.008) 4104.06 ng****response 1403241**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.25
183.00	13.20	12.24
0.00	0.00	0.00