


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040721\
 Data File : BE101220.D
 Acq On : 7 Apr 2021 8:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE040621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 07 10:22:45 2021

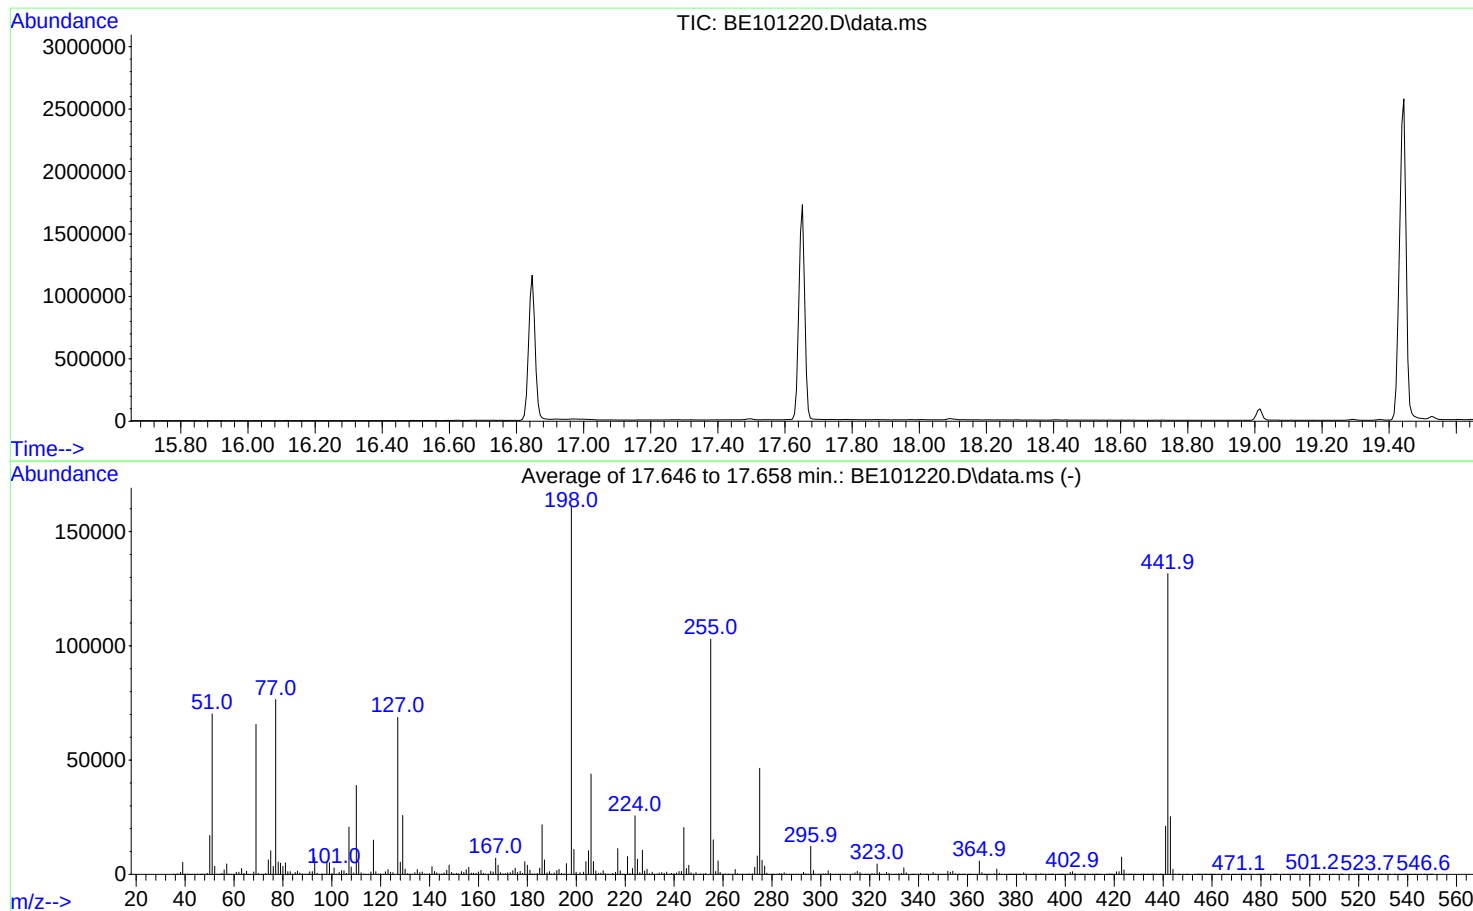




AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.6	70238	PASS
68	69	0.00	2	1.6	1025	PASS
69	198	0.00	100	40.8	65633	PASS
70	69	0.00	2	0.5	325	PASS
127	198	10	80	42.7	68727	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	161016	PASS
199	198	5	9	6.8	10949	PASS
275	198	10	60	28.9	46462	PASS
365	198	1	100	3.6	5850	PASS
441	198	0.01	100	13.1	21052	PASS
442	442	50	100	100.0	131648	PASS
443	442	15	24	19.2	25256	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040721\
 Data File : BE101220.D
 Acq On : 7 Apr 2021 8:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Quant Time: Apr 07 10:17:28 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 31 10:54:22 2021
 Response via : Initial Calibration

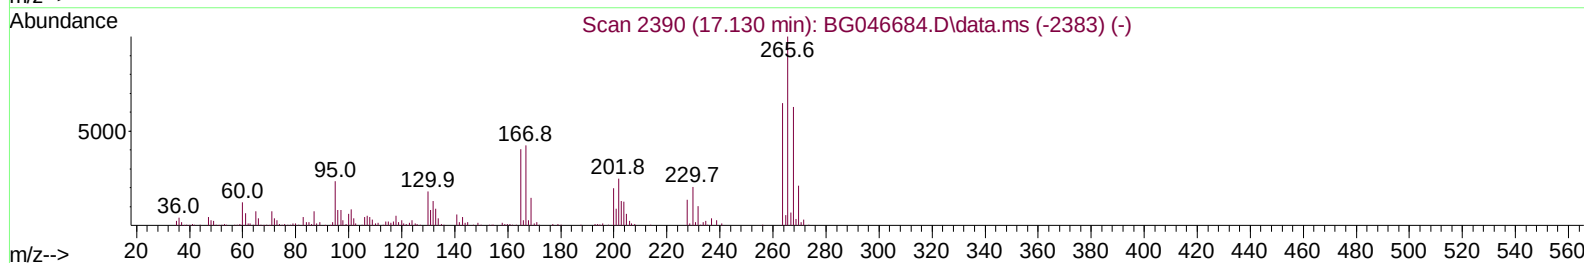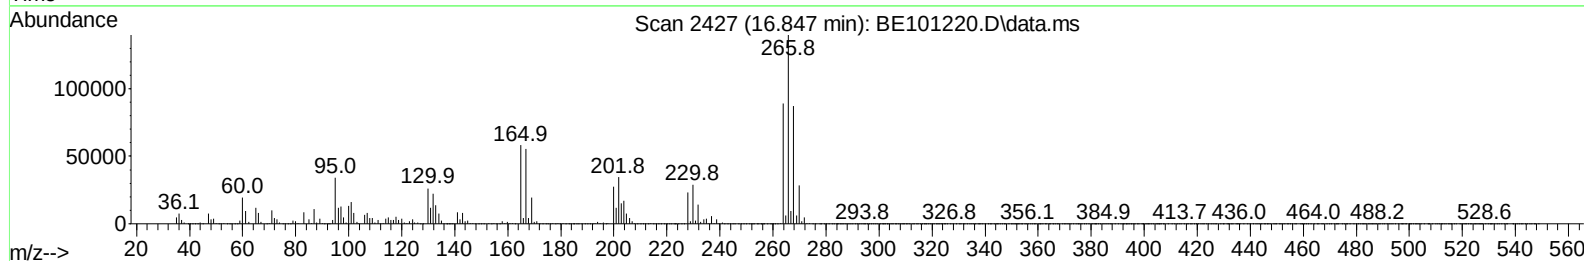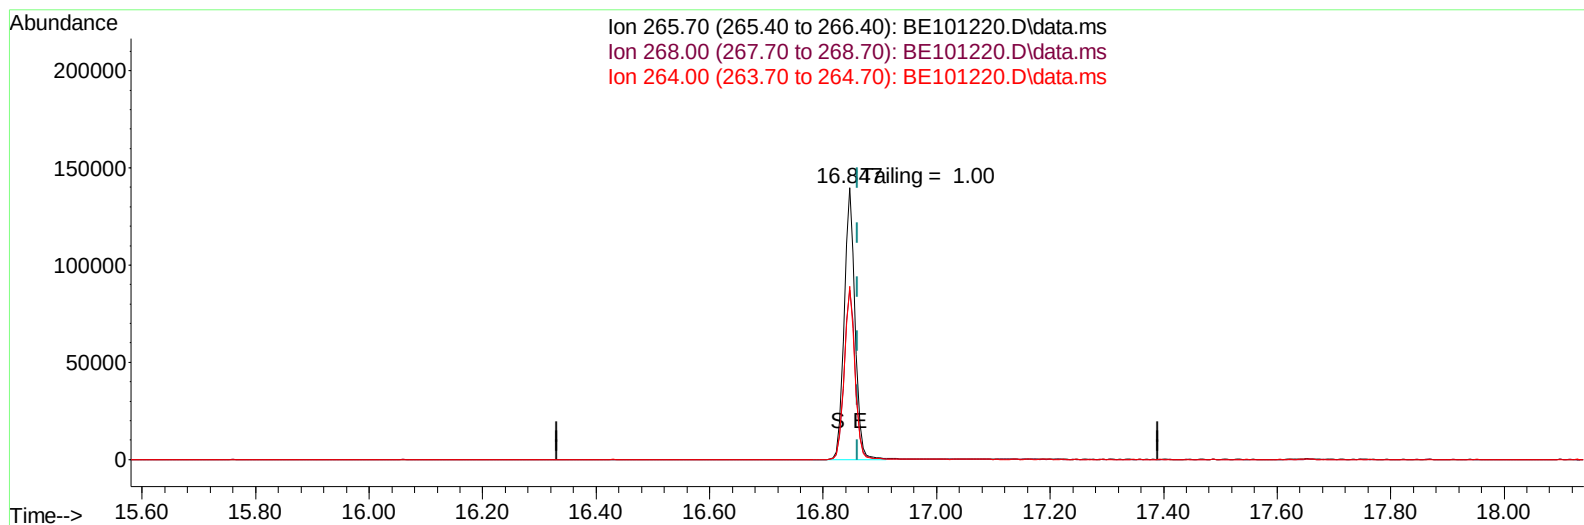

TIC: BE101220.D\data.ms

(70) Pentachlorophenol (C)

16.847min (-0.013) 1698185.03 ng




response 186577

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.40
264.00	61.60	63.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040721\
Data File : BE101220.D
Acq On : 7 Apr 2021 8:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Apr 07 10:17:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 10:54:22 2021
Response via : Initial Calibration

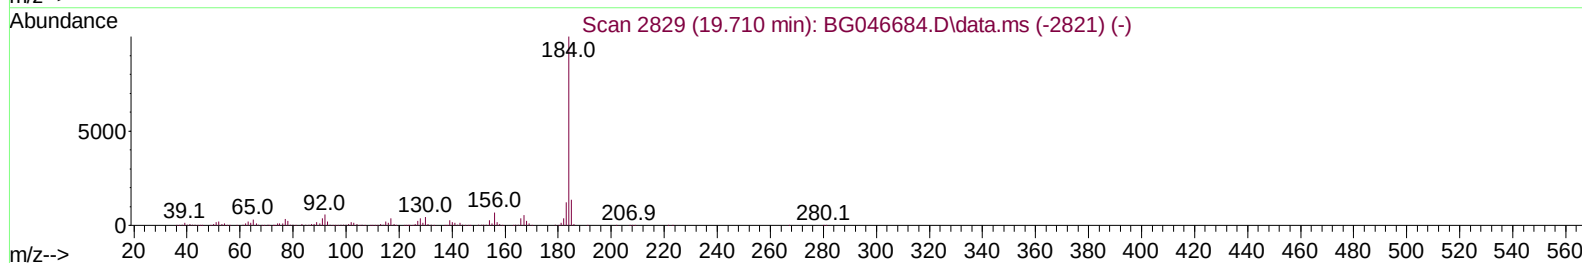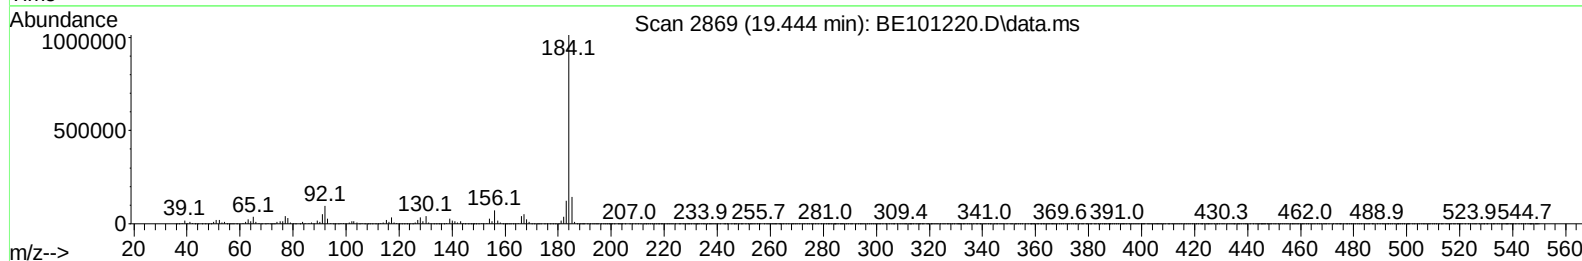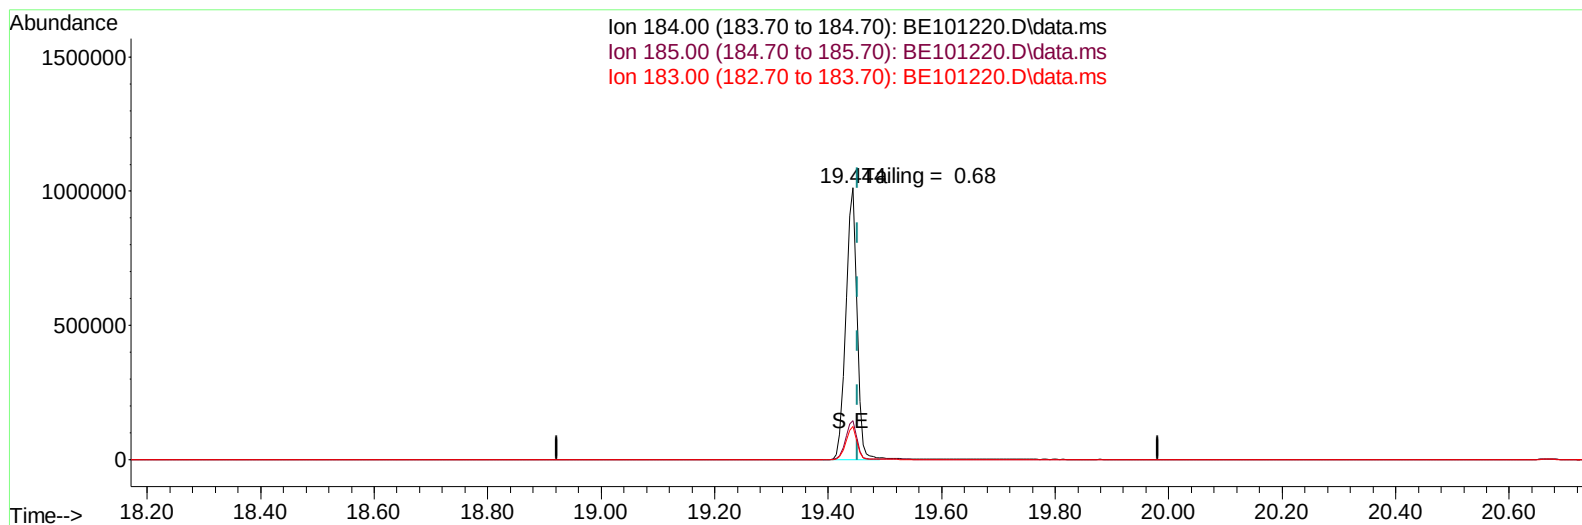

TIC: BE101220.D\data.ms

(77) Benzidine

19.444min (-0.008) 4104.06 ng

response 1403241

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.25
183.00	13.20	12.24
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_E
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
4/7/2021	BNA_E	BE101220.D
Compound Name	Response	Retention Time
DDT	744471	20.672
DDD	1589	20.231
DDE	824	19.726
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2413	746884	0.32

Instrument :
BNA_E
ClientSampleId :
DFTPP