

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE041219\
 Data File : BE099316.D
 Acq On : 12 Apr 2019 18:29
 Operator : JU/SJ
 Sample : K2366-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SA-SW124-20190409

Quant Time: Apr 12 20:33:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE040219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 02 17:16:42 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	4170	0.40	ng	-0.02
7) Naphthalene-d8	10.61	136	15327	0.40	ng	-0.01
13) Acenaphthene-d10	14.46	164	10178	0.40	ng	-0.03
19) Phenanthrene-d10	17.19	188	32211	0.40	ng	-0.03
27) Chrysene-d12	21.37	240	44886	0.40	ng	-0.02
34) Perylene-d12	23.85	264	44395	0.40	ng	-0.04
System Monitoring Compounds						
4) 2-Fluorophenol	5.40	112	402	0.04	ng	-0.01
5) Phenol-d6	6.98	99	129	0.01	ng	-0.01
8) Nitrobenzene-d5	8.96	82	2482	0.24	ng	-0.03
11) 2-Methylnaphthalene-d10	12.19	152	7956	0.30	ng	-0.03
14) 2,4,6-Tribromophenol	15.94	330	333	0.07	ng	-0.01
15) 2-Fluorobiphenyl	13.09	172	15286	0.38	ng	-0.01
25) Fluoranthene-d10	19.21	212	142667	0.34	ng	-0.03
29) Terphenyl-d14	19.81	244	33466	0.41	ng	-0.02
Target Compounds						Qvalue
32) Bis(2-ethylhexyl)phthalate	21.27	149	23793	0.132	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE041219\
Data File : BE099316.D
Acq On : 12 Apr 2019 18:29
Operator : JU/SJ
Sample : K2366-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SA-SW124-20190409

Quant Time: Apr 12 20:33:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE040219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 02 17:16:42 2019
Response via : Initial Calibration

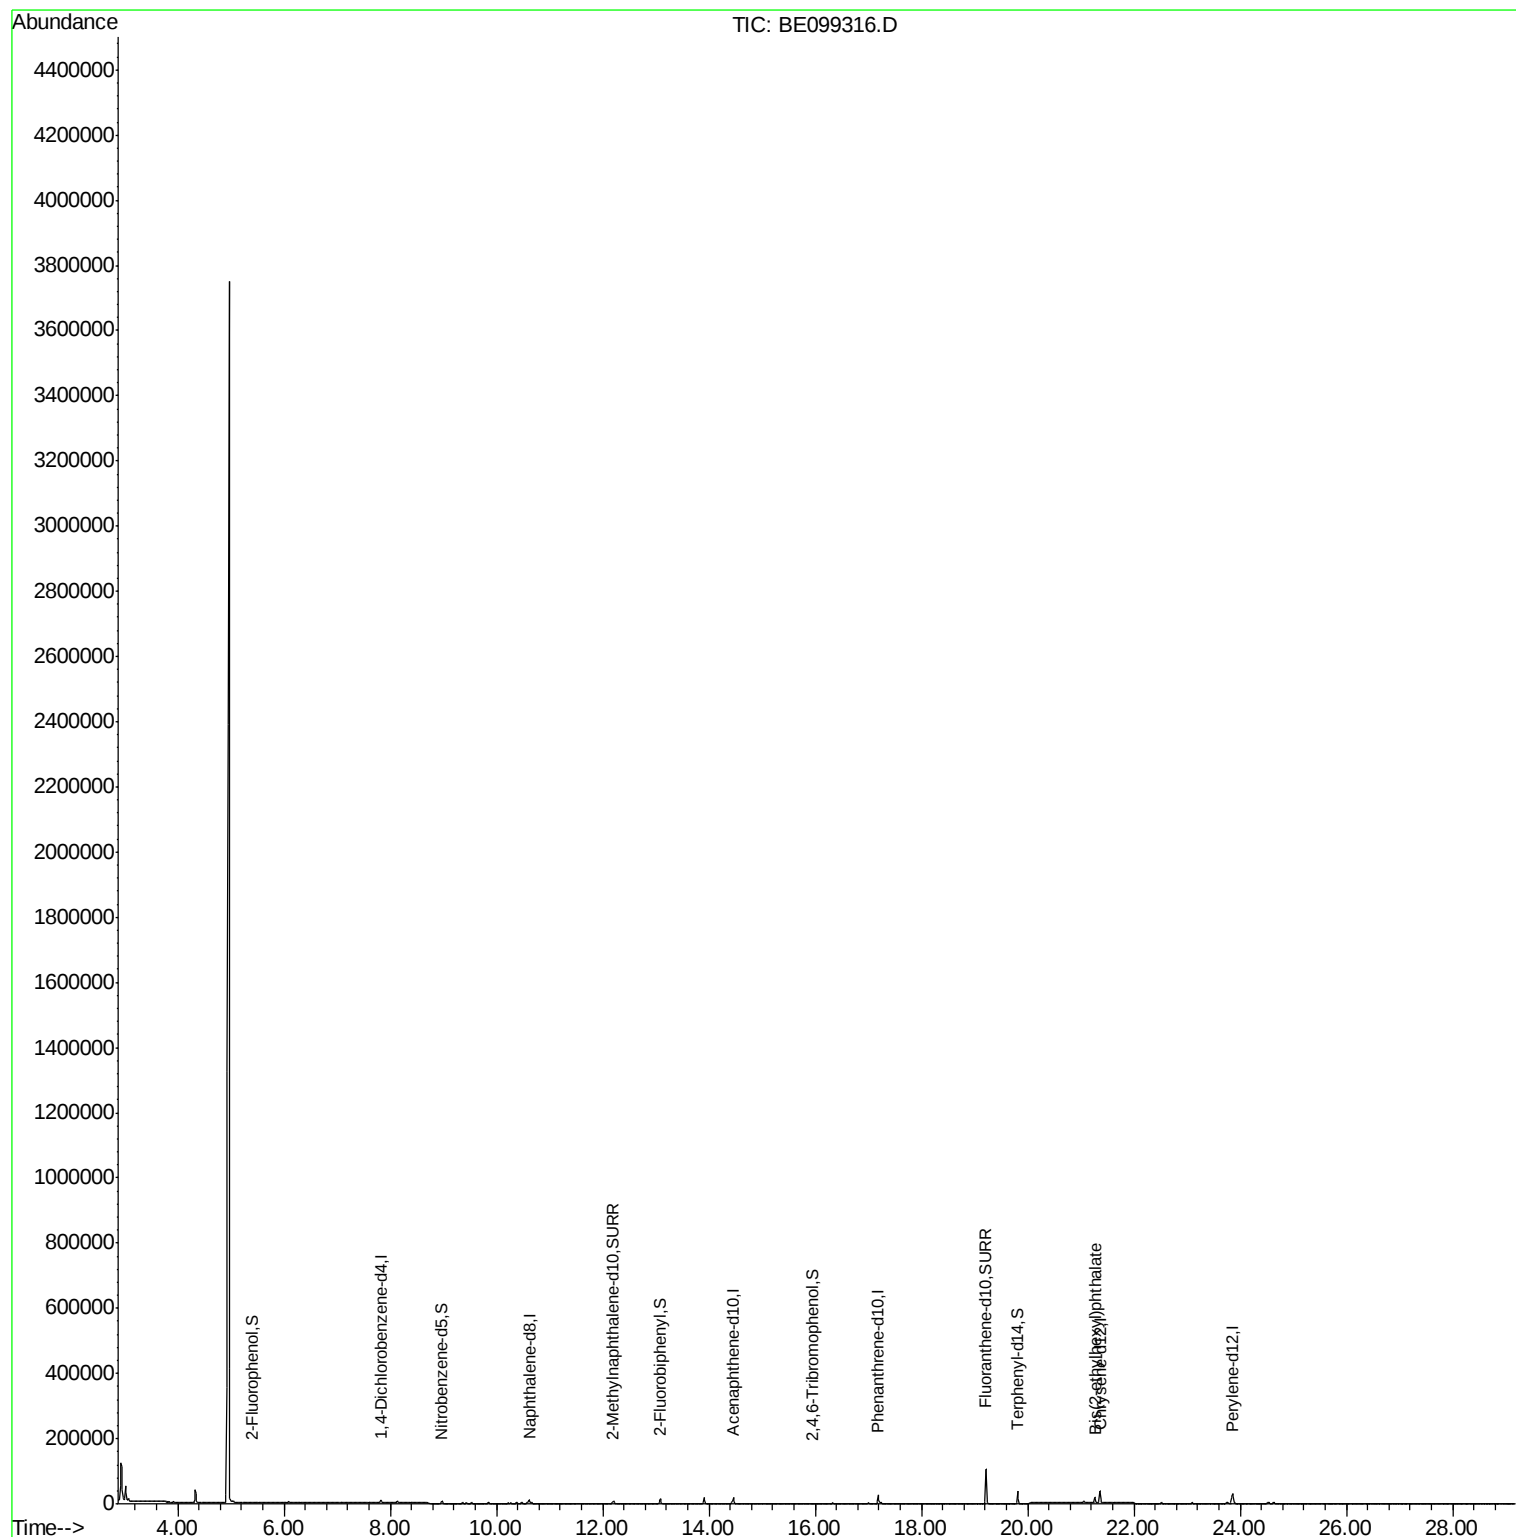

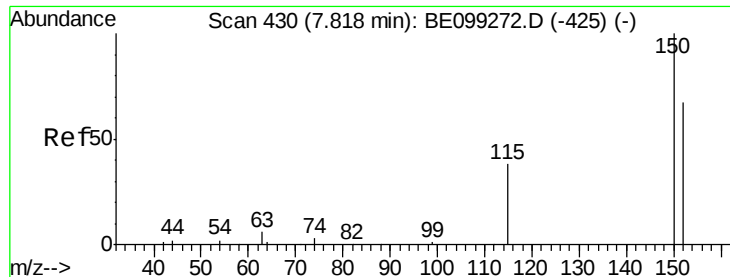

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.82 min Scan# 430

Delta R.T. -0.02 min

Lab File: BE099316.D

Acq: 12 Apr 2019 18:29

Instrument :

BNA_E

ClientSampleId :

SA-SW124-20190409


Tgt Ion:152 Resp: 4170

Ion Ratio Lower Upper

152 100

150 143.6 112.8 169.2




115 57.7 45.1 67.7

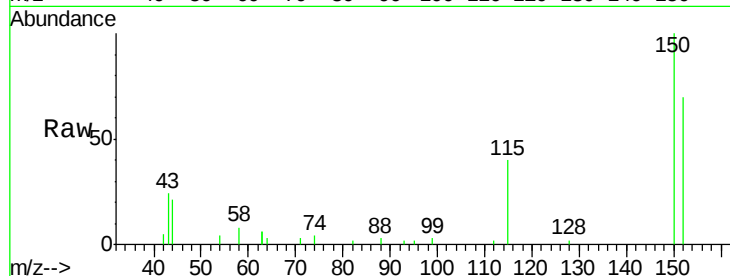

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

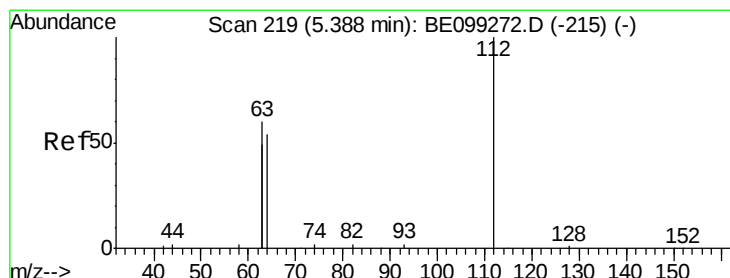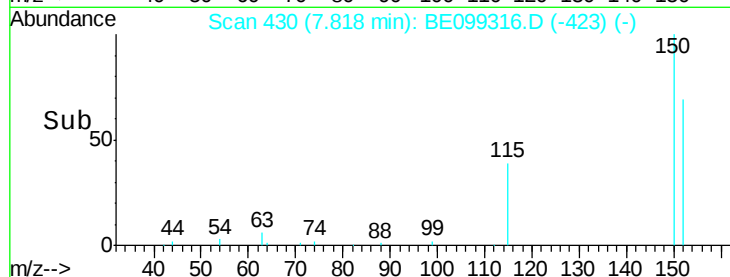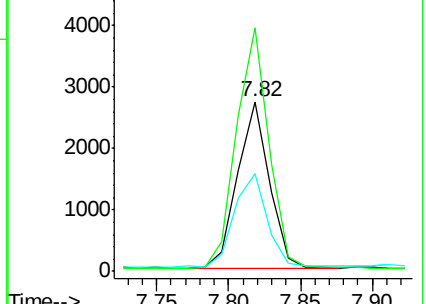

#4

2-Fluorophenol

Concen: 0.036 ng

RT: 5.40 min Scan# 220

Delta R.T. -0.01 min

Lab File: BE099316.D

Acq: 12 Apr 2019 18:29


Tgt Ion:112 Resp: 402

Ion Ratio Lower Upper

112 100

64 41.0 46.2 69.2#



63 94.8 89.9 134.9

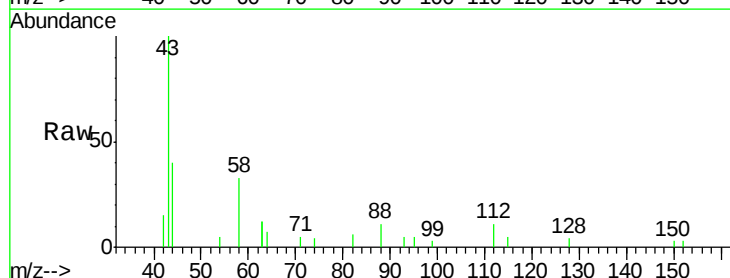


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

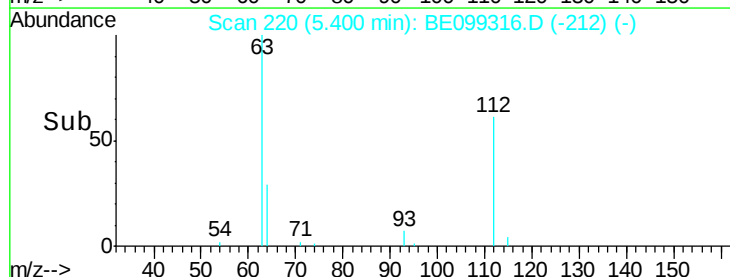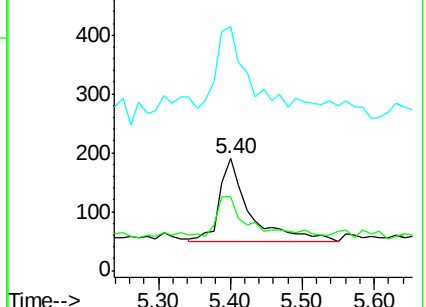

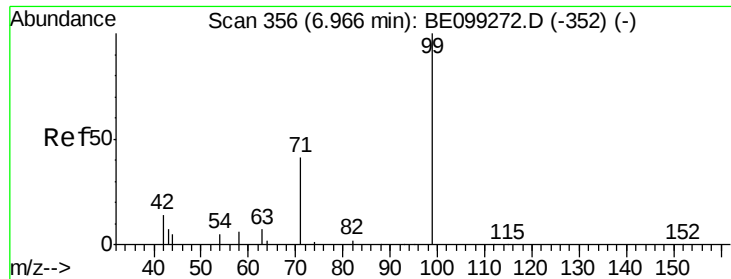

#5

Phenol-d6

Concen: 0.008 ng

RT: 6.98 min Scan# 357

Delta R.T. -0.01 min

Lab File: BE099316.D

Acq: 12 Apr 2019 18:29

Instrument :

BNA_E

ClientSampleId :

SA-SW124-20190409


Tgt Ion: 99 Resp: 129

Ion Ratio Lower Upper

99 100

42 93.0 12.4 18.6#




71 152.7 28.4 42.6#

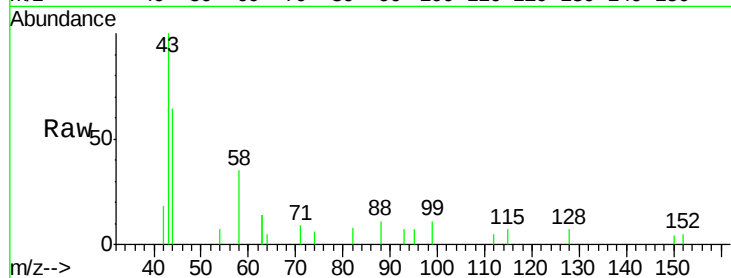

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

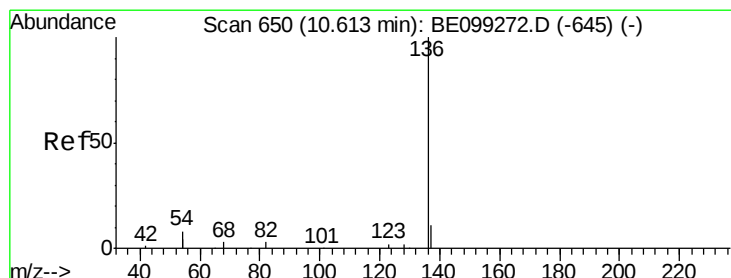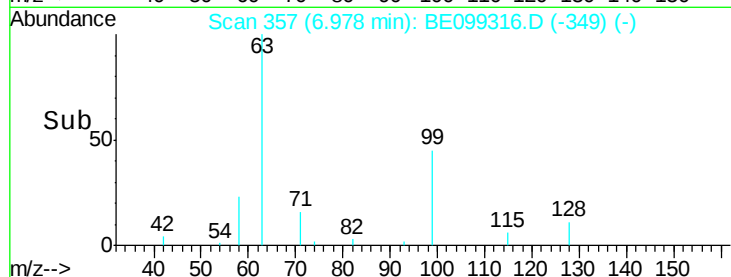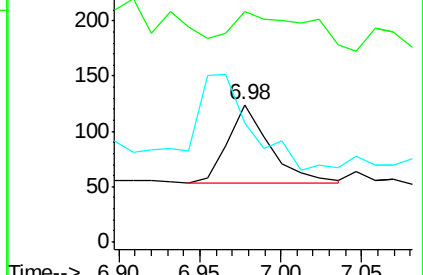

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.61 min Scan# 650

Delta R.T. -0.01 min

Lab File: BE099316.D

Acq: 12 Apr 2019 18:29

Tgt Ion: 136 Resp: 15327


Ion Ratio Lower Upper

136 100

137 10.8 8.7 13.1

54 15.3 18.7 28.1#

68 4.7 5.2 7.8#


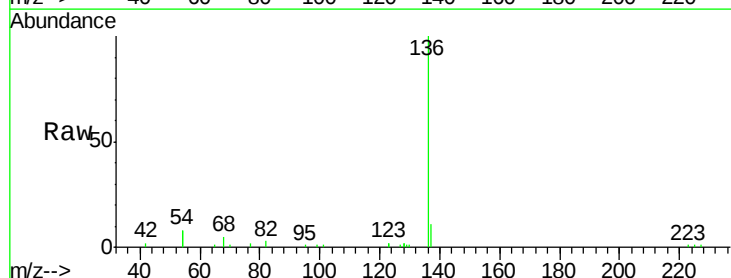



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

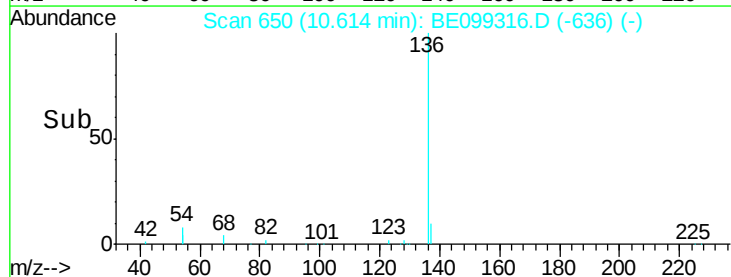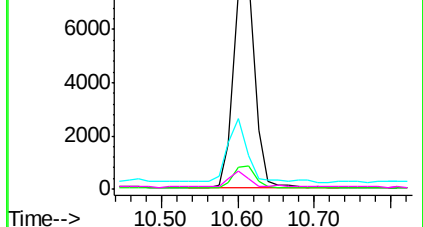

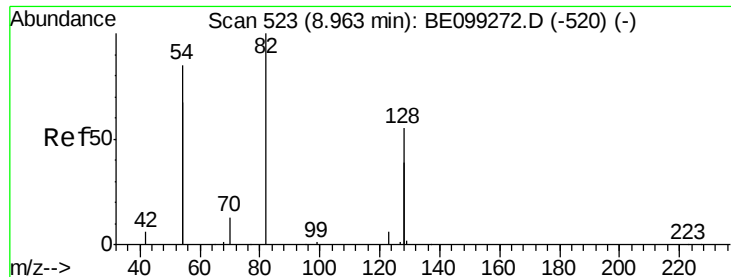

#8

Nitrobenzene-d5

Concen: 0.236 ng

RT: 8.96 min Scan# 523

Delta R.T. -0.03 min

Lab File: BE099316.D

Acq: 12 Apr 2019 18:29

Instrument :

BNA_E

ClientSampleId :

SA-SW124-20190409


Tgt Ion: 82 Resp: 2482

Ion Ratio Lower Upper

82 100

128 109.5 107.5 161.3


54 166.1 106.3 159.5#

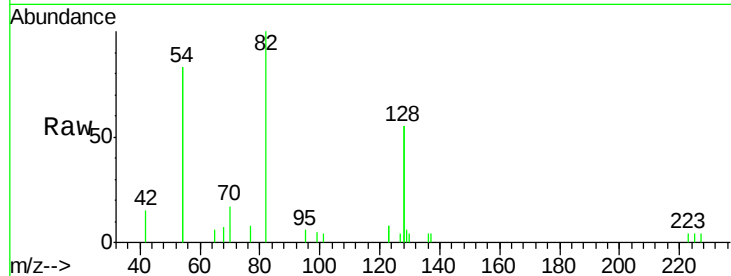



Abundance Ion 82.00 (81.70 to 82.70): BE099316.D (-517) (-)

Ion 128.00 (127.70 to 128.70): BE099316.D (-517) (-)

Ion 54.00 (53.70 to 54.70): BE099316.D (-517) (-)

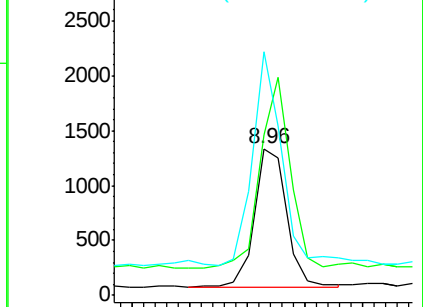

Time--> 8.85 8.90 8.95 9.00 9.05

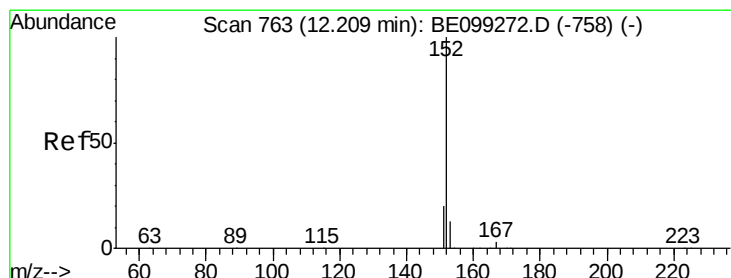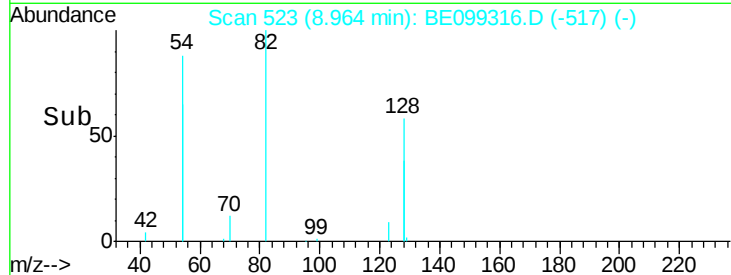

#11

2-Methylnaphthalene-d10

Concen: 0.297 ng

RT: 12.19 min Scan# 762

Delta R.T. -0.03 min

Lab File: BE099316.D


Acq: 12 Apr 2019 18:29

Tgt Ion: 152 Resp: 7956

Ion Ratio Lower Upper


152 100

151 19.0 15.0 22.6

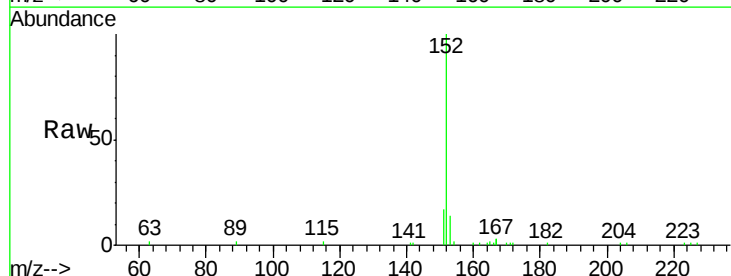



Abundance Ion 152.00 (151.70 to 152.70): BE099316.D (-757) (-)

Ion 151.00 (150.70 to 151.70): BE099316.D (-757) (-)

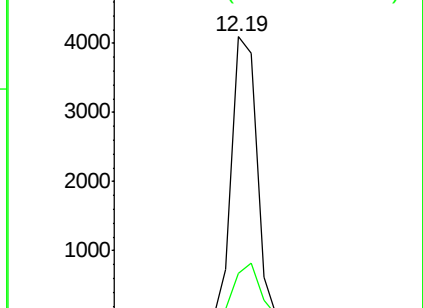

Time--> 12.10 12.20 12.30

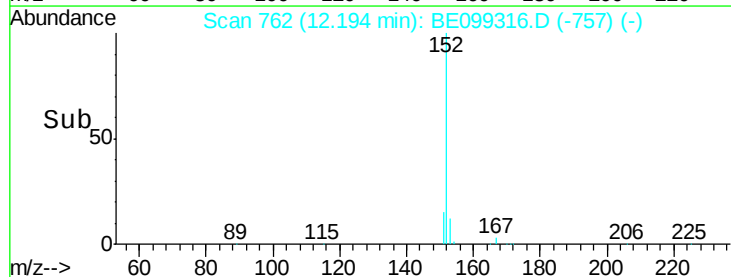

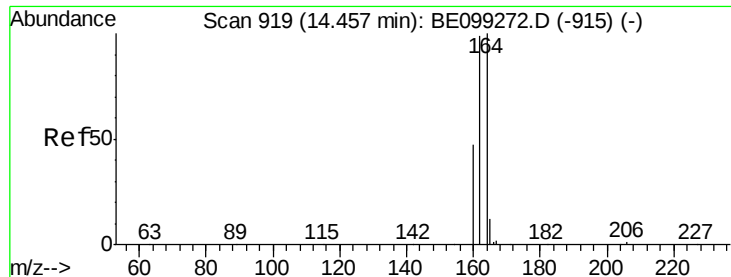

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.46 min Scan# 919

Delta R.T. -0.03 min

Lab File: BE099316.D

Acq: 12 Apr 2019 18:29

Instrument :

BNA_E

ClientSampleId :

SA-SW124-20190409


Tgt Ion:164 Resp: 10178

Ion Ratio Lower Upper

164 100

162 101.1 79.2 118.8




160 46.1 36.7 55.1

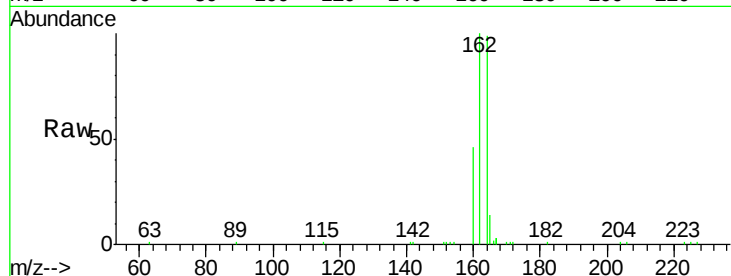

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

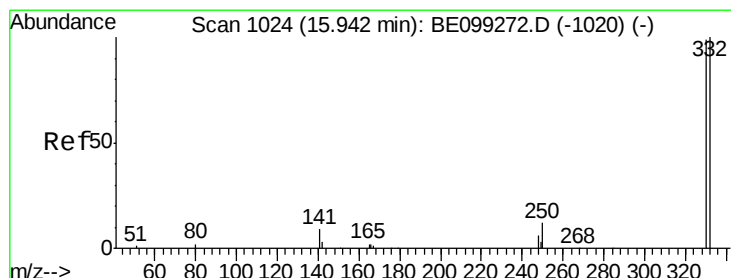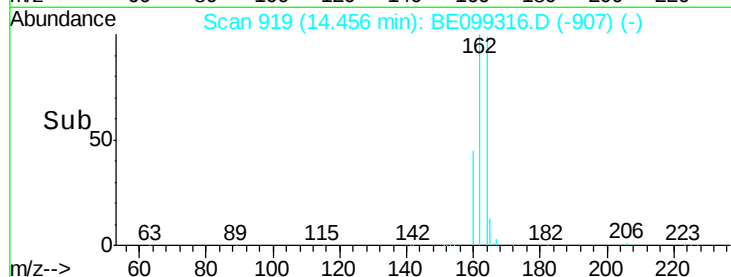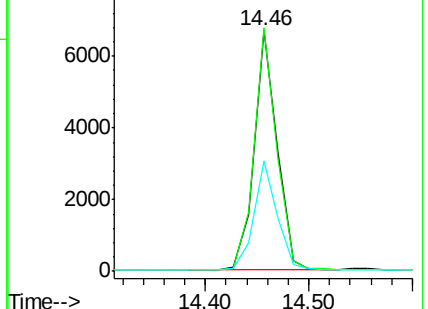

#14

2,4,6-Tribromophenol

Concen: 0.071 ng

RT: 15.94 min Scan# 1024

Delta R.T. -0.01 min

Lab File: BE099316.D

Acq: 12 Apr 2019 18:29


Tgt Ion:330 Resp: 333

Ion Ratio Lower Upper

330 100

332 108.1 71.3 106.9#



141 40.8 21.7 32.5#

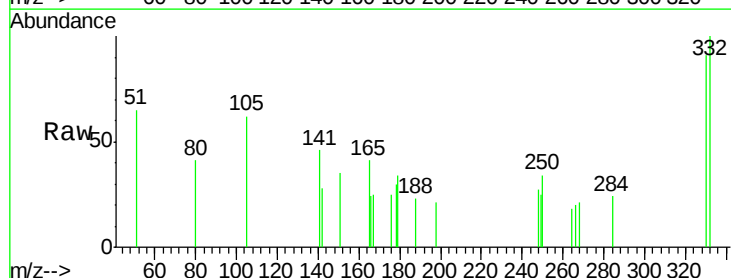


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



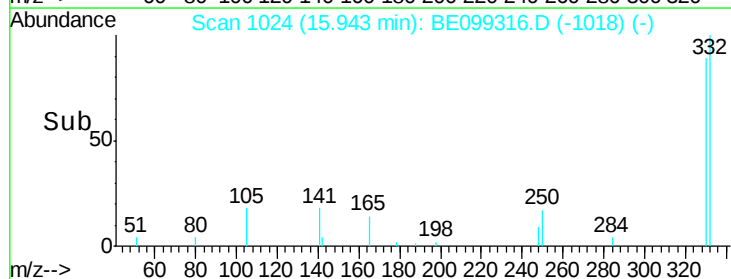
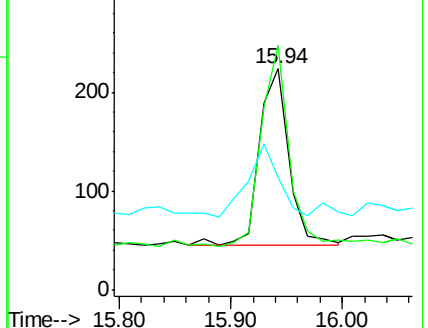


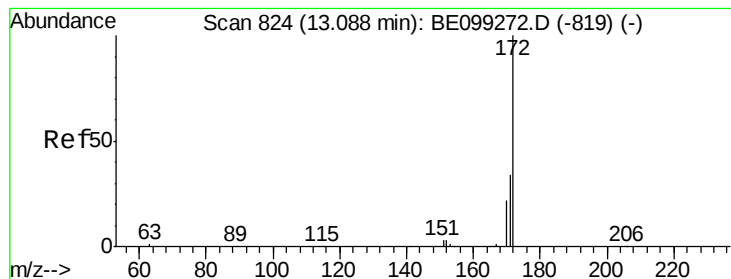

#15
2-Fluorobiphenyl
Concen: 0.382 ng
RT: 13.09 min Scan# 824
Delta R.T. -0.01 min
Lab File: BE099316.D
Acq: 12 Apr 2019 18:29




Instrument :
BNA_E
ClientSampleId :
SA-SW124-20190409


Tgt Ion:172 Resp: 15286
Ion Ratio Lower Upper
172 100
171 34.7 27.4 41.0
170 22.5 19.1 28.7

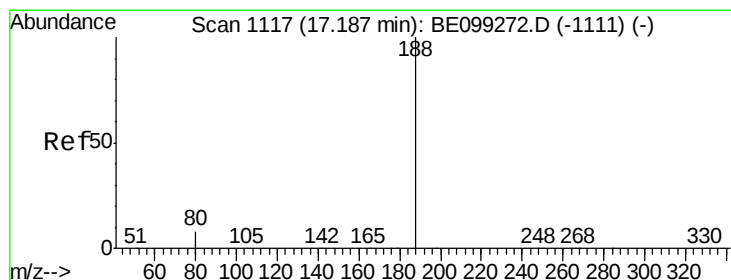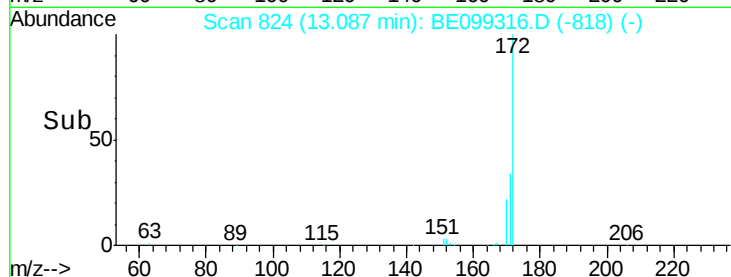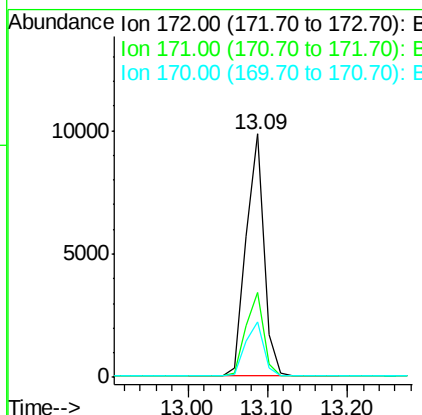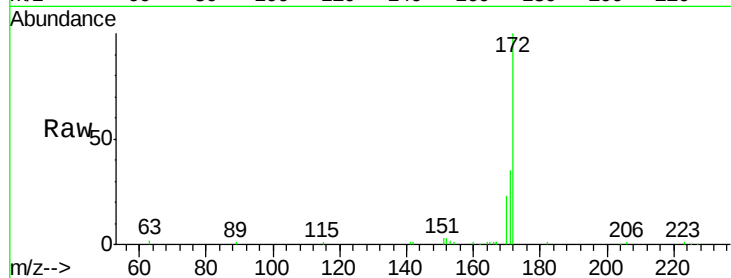

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.19 min Scan# 1117
Delta R.T. -0.03 min
Lab File: BE099316.D
Acq: 12 Apr 2019 18:29

Tgt Ion:188 Resp: 32211
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.7 4.5 6.7#

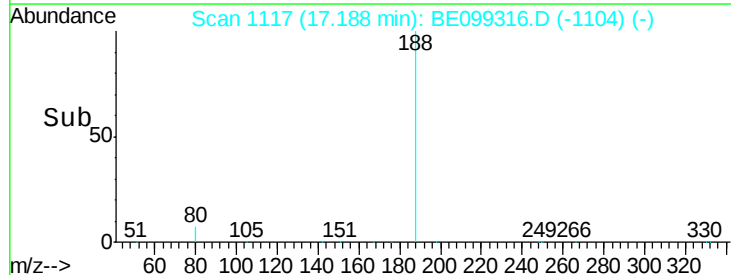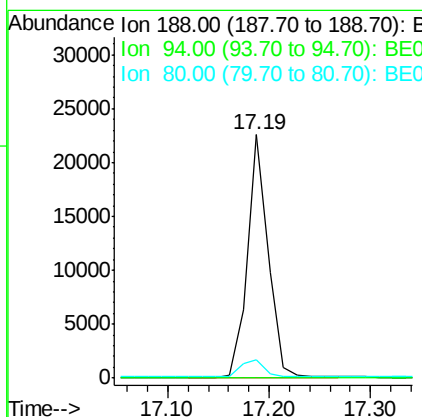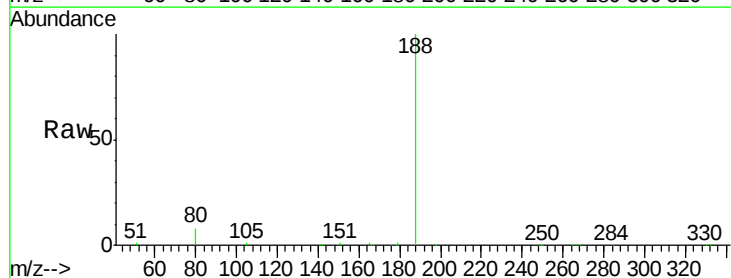

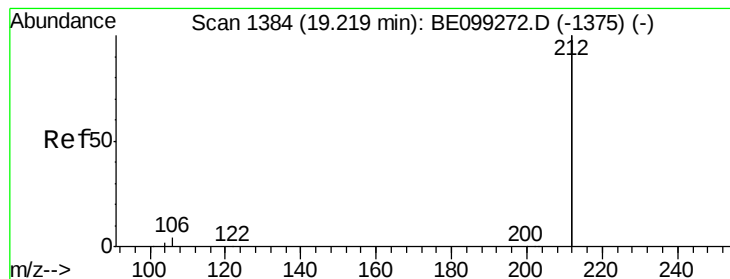

#25

Fluoranthene-d10

Concen: 0.336 ng

RT: 19.21 min Scan# 1383

Delta R.T. -0.03 min

Lab File: BE099316.D

Acq: 12 Apr 2019 18:29

Instrument :

BNA_E

ClientSampleId :

SA-SW124-20190409


Tgt Ion:212 Resp: 142667

Ion Ratio Lower Upper

212 100

106 2.1 1.8 2.8




104 1.2 1.1 1.7

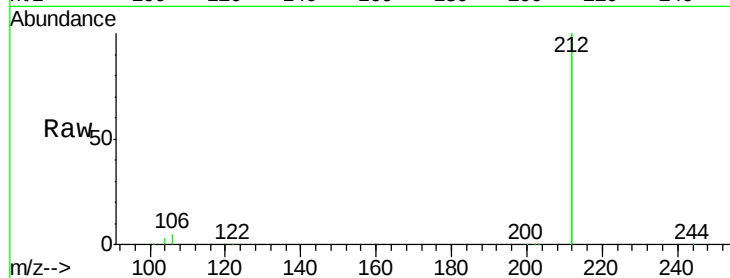

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

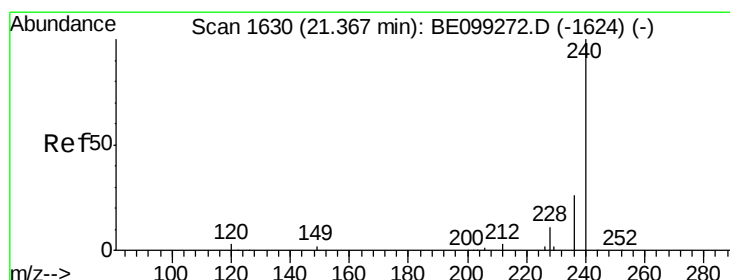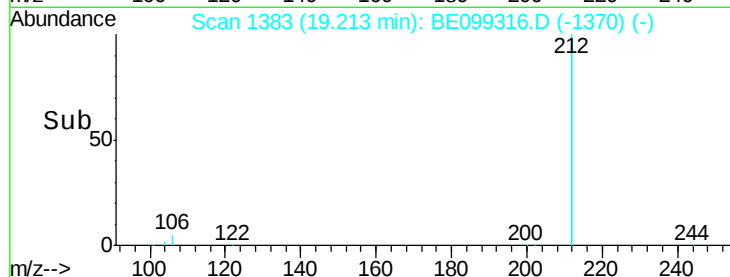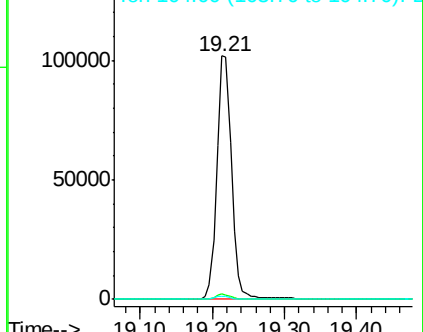

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.37 min Scan# 1630

Delta R.T. -0.02 min

Lab File: BE099316.D

Acq: 12 Apr 2019 18:29


Tgt Ion:240 Resp: 44886

Ion Ratio Lower Upper

240 100

120 2.9 2.6 3.8



236 26.5 20.9 31.3

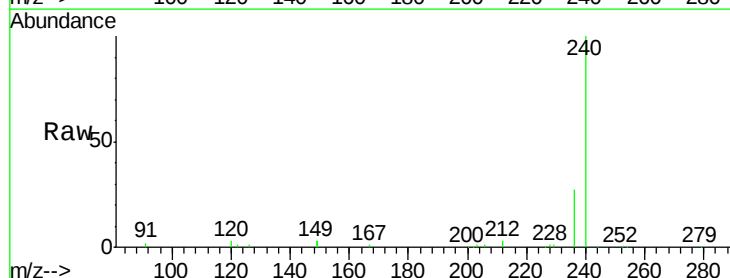


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

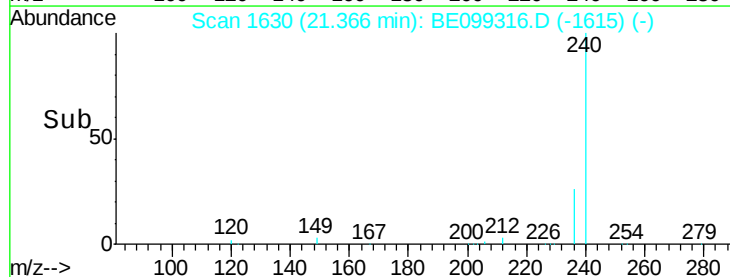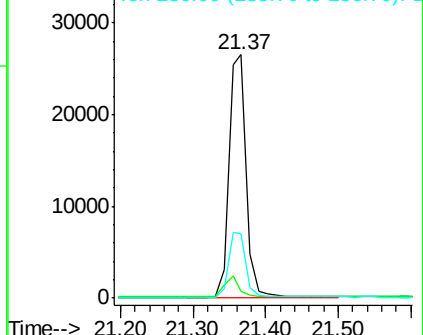

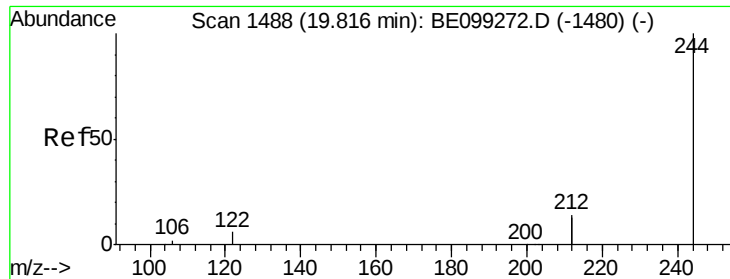

#29

Terphenyl-d14

Concen: 0.409 ng

RT: 19.81 min Scan# 1487

Delta R.T. -0.02 min

Lab File: BE099316.D

Acq: 12 Apr 2019 18:29

Instrument :

BNA_E

ClientSampleId :

SA-SW124-20190409


Tgt Ion:244 Resp: 33466

Ion Ratio Lower Upper

244 100

212 31.5 22.7 34.1




122 7.6 5.8 8.6

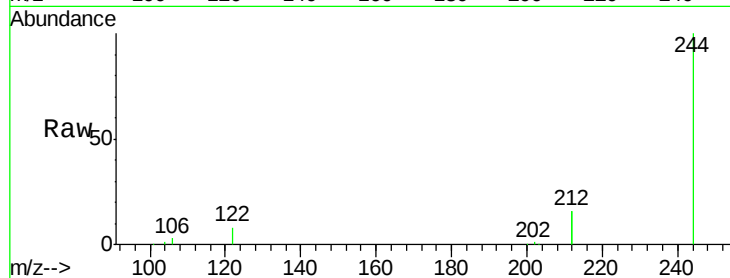

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

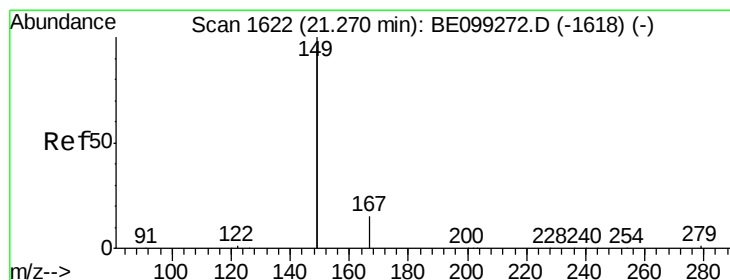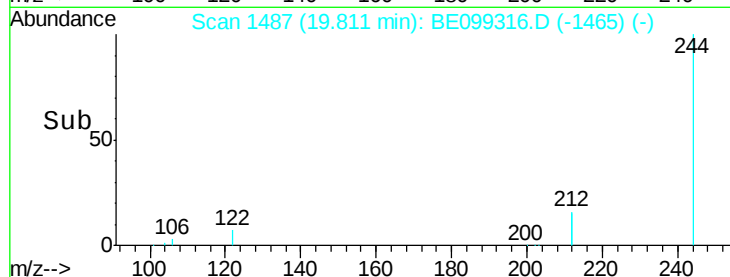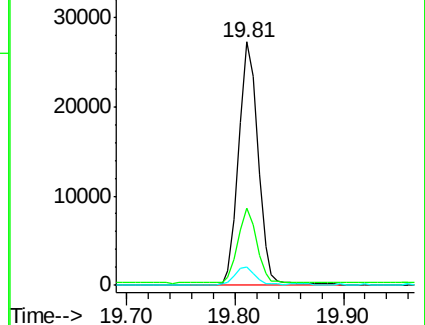

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.132 ng

RT: 21.27 min Scan# 1622

Delta R.T. -0.02 min

Lab File: BE099316.D

Acq: 12 Apr 2019 18:29


Tgt Ion:149 Resp: 23793

Ion Ratio Lower Upper

149 100

167 7.7 5.9 8.9



279 1.3 1.0 1.6



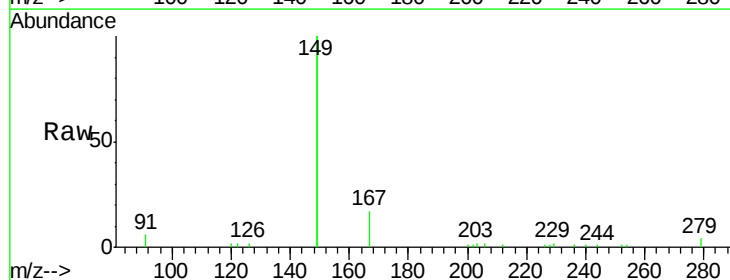


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

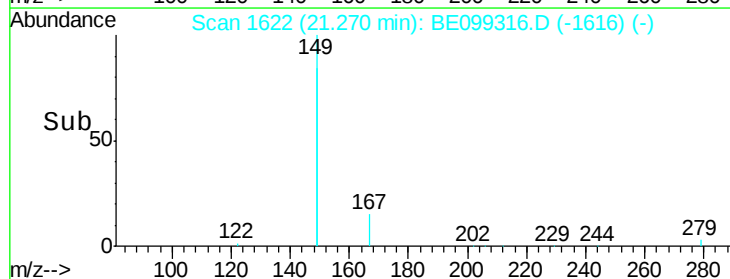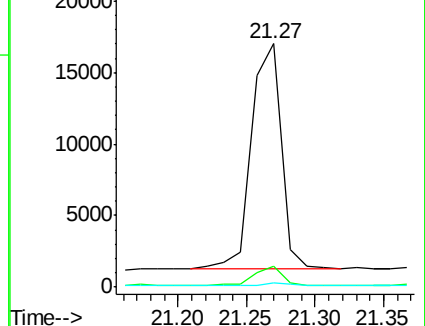

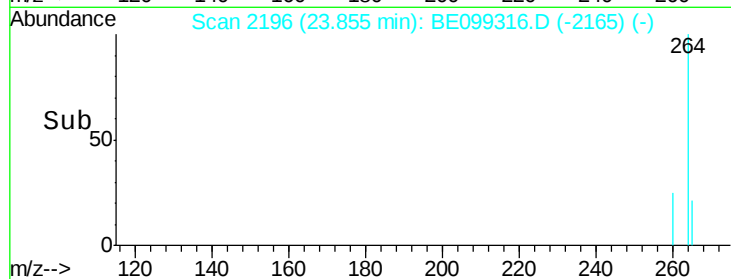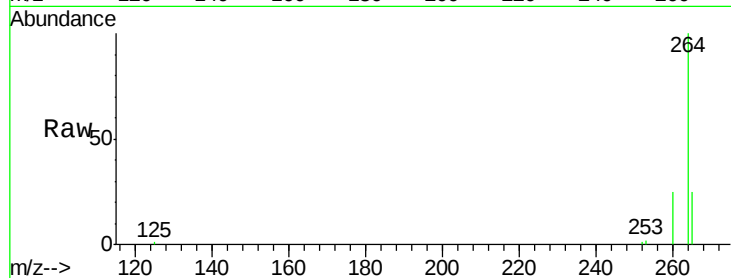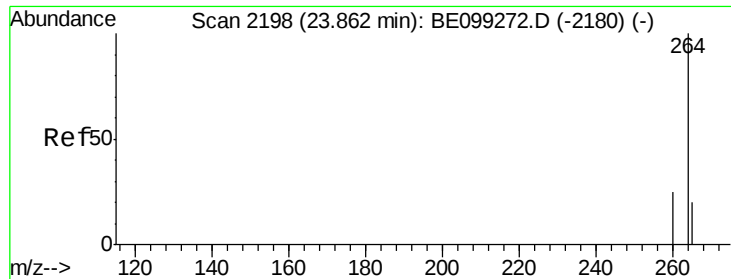

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.85 min Scan# 2196

Delta R.T. -0.04 min

Lab File: BE099316.D

Acq: 12 Apr 2019 18:29

Instrument :

BNA_E

ClientSampleId :

SA-SW124-20190409

Tgt Ion: 264 Resp: 44395

Ion Ratio Lower Upper

264 100

260 25.1 18.2 27.2

265 24.6 21.8 32.8

