


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE041219\
Data File : BE099308.D
Acq On : 12 Apr 2019 13:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE040219.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 12 20:31:12 2019

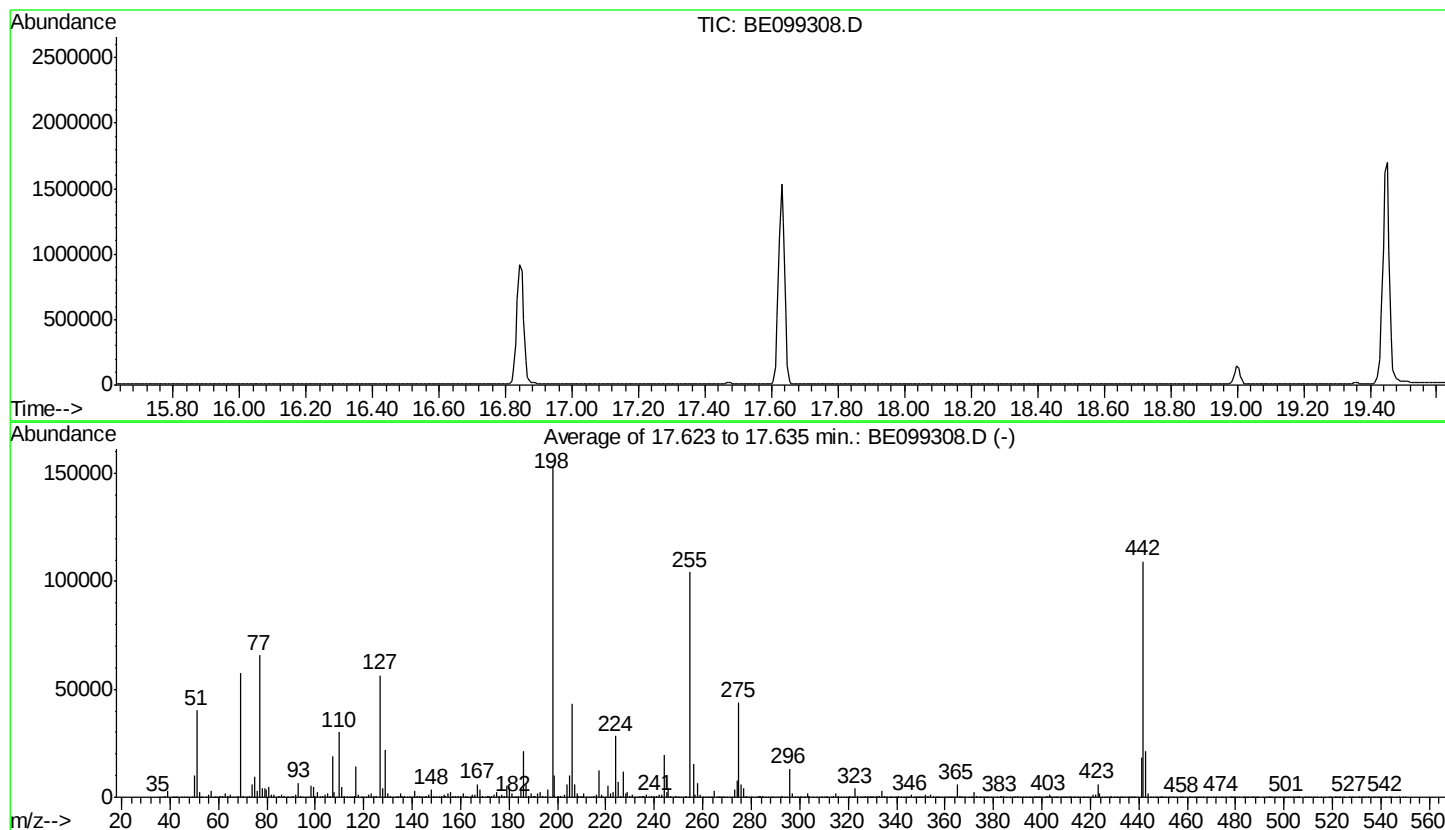

AutoFind: Scans 2559, 2560, 2561; Background Corrected with Scan 2551

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.1	40085	PASS
68	69	0.00	2	1.0	564	PASS
69	198	0.00	100	37.5	57571	PASS
70	69	0.00	2	0.6	323	PASS
127	198	10	80	36.8	56494	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	153704	PASS
199	198	5	9	6.7	10267	PASS
275	198	10	60	28.6	43898	PASS
365	198	1	100	3.8	5859	PASS
441	198	0.01	100	11.9	18236	PASS
442	198	50	100	71.1	109309	PASS
443	442	15	24	19.4	21205	PASS