
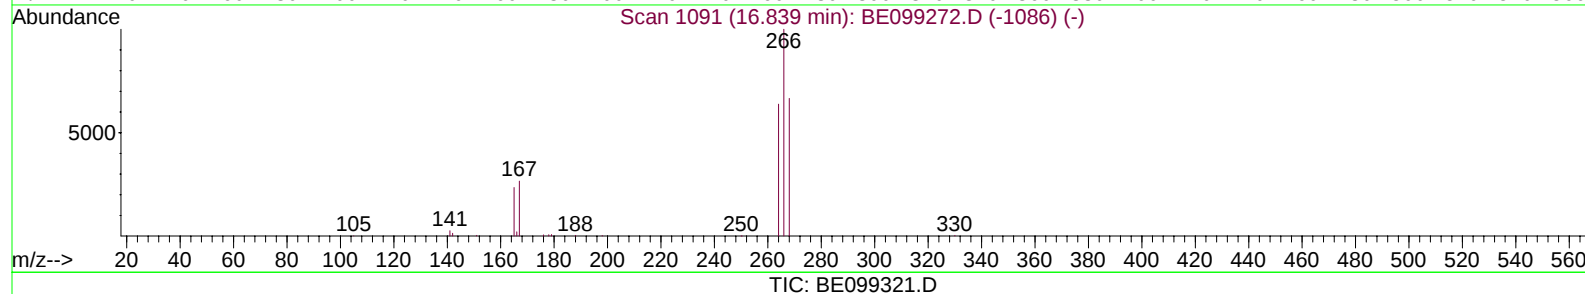
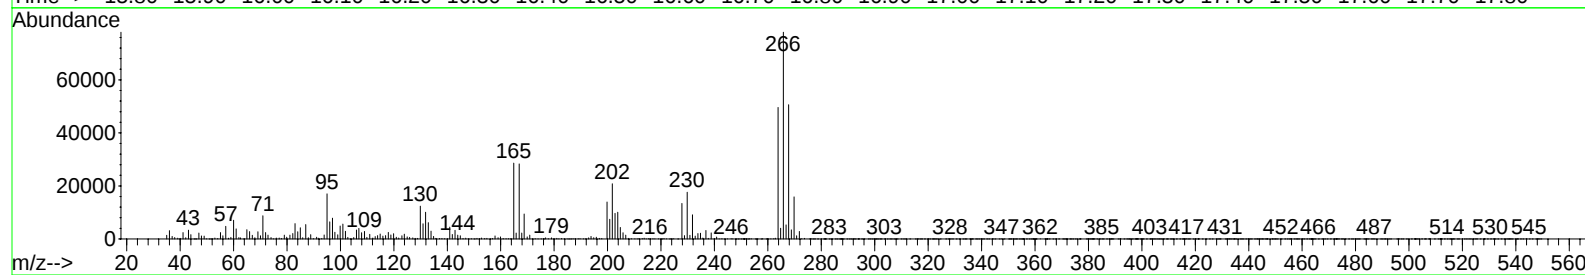


```
Data Path   : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE041519\  
Data File   : BE099321.D  
Acq On      : 15 Apr 2019      8:55  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Apr 15 18:13:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE040219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 02 17:16:42 2019
Response via : Initial Calibration

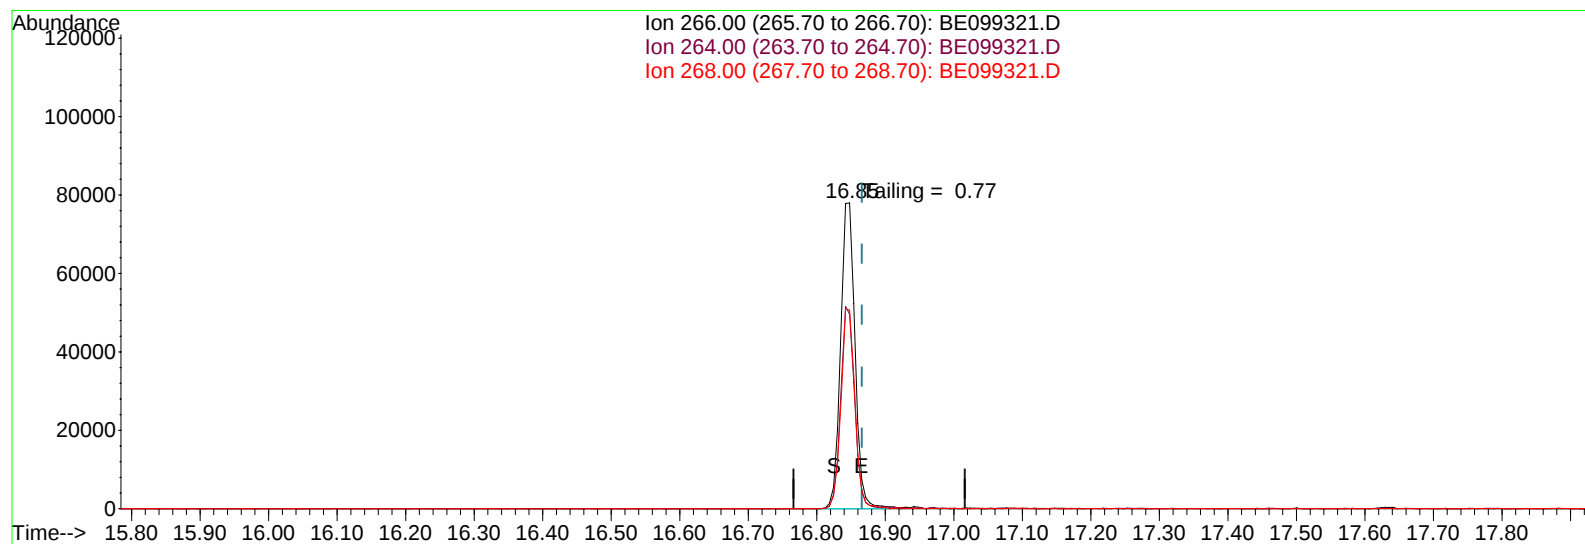

(22) Pentachlorophenol

16.848min (-0.018) 2163.00ng

```
response 114077
```

Ion	Exp%	Act%
266.00	100	100
264.00	68.00	63.66
268.00	76.60	64.94
0.00	0.00	0.00