

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE041819\
 Data File : BE099335.D
 Acq On : 18 Apr 2019 12:20
 Operator : JU/SJ
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2

Quant Time: Apr 18 14:02:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE041819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 13:54:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	3929	0.40	ng	0.00
7) Naphthalene-d8	10.60	136	14930	0.40	ng	0.00
13) Acenaphthene-d10	14.46	164	10580	0.40	ng	0.00
19) Phenanthrene-d10	17.19	188	29303	0.40	ng	0.00
27) Chrysene-d12	21.37	240	37224	0.40	ng	0.00
34) Perylene-d12	23.86	264	32616	0.40	ng	0.00

System Monitoring Compounds

4) 2-Fluorophenol	5.39	112	30958	2.96	ng	0.00
5) Phenol-d6	6.97	99	45462	3.17	ng	0.00
8) Nitrobenzene-d5	8.96	82	40623	3.96	ng	0.00
11) 2-Methylnaphthalene-d10	12.20	152	87063	3.34	ng	0.00
14) 2,4,6-Tribromophenol	15.94	330	16136	3.31	ng	0.00
15) 2-Fluorobiphenyl	13.09	172	133592	3.21	ng	0.00
25) Fluoranthene-d10	19.22	212	1193886	3.09	ng	0.00
29) Terphenyl-d14	19.82	244	239302	3.52	ng	0.00

Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.31	88	16777	3.134	ng	98
3) n-Nitrosodimethylamine	3.64	42	11147	3.527	ng	# 95
6) bis(2-Chloroethyl)ether	7.24	93	41200	3.201	ng	96
9) Naphthalene	10.65	128	524817	3.232	ng	99
10) Hexachlorobutadiene	10.94	225	33490	3.174	ng	99
12) 2-Methylnaphthalene	12.27	142	92700	3.355	ng	98
16) Acenaphthylene	14.18	152	170479	3.401	ng	99
17) Acenaphthene	14.51	154	97374	3.292	ng	97
18) Fluorene	15.49	166	139947	3.275	ng	99
20) 4-Bromophenyl-phenylether	16.38	248	55625	3.344	ng	96
21) Hexachlorobenzene	16.49	284	52668	3.326	ng	99
22) Pentachlorophenol	16.84	266	19339	2.941	ng	95
23) Phenanthrene	17.23	178	252752	3.333	ng	100
24) Anthracene	17.32	178	239374	3.347	ng	99
26) Fluoranthene	19.25	202	357678	3.196	ng	99
28) Pyrene	19.61	202	357087	3.632	ng	99
30) Benzo(a)anthracene	21.34	228	365841	3.122	ng	99
31) Chrysene	21.40	228	381784	3.322	ng	99
32) Bis(2-ethylhexyl)phthalate	21.27	149	374295	2.505	ng	100
33) Indeno(1,2,3-cd)pyrene	26.49	276	379461	2.889	ng	99
35) Benzo(b)fluoranthene	23.09	252	339246	3.486	ng	99
36) Benzo(k)fluoranthene	23.14	252	336406	3.552	ng	98
37) Benzo(a)pyrene	23.74	252	306936	3.355	ng	99
38) Dibenzo(a,h)anthracene	26.52	278	315852	3.472	ng	98
39) Benzo(g,h,i)perylene	27.30	276	313985	3.463	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE041819\
 Data File : BE099335.D
 Acq On : 18 Apr 2019 12:20
 Operator : JU/SJ
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 SSTDICC3.2

Quant Time: Apr 18 14:02:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE041819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 18 13:54:27 2019
 Response via : Initial Calibration




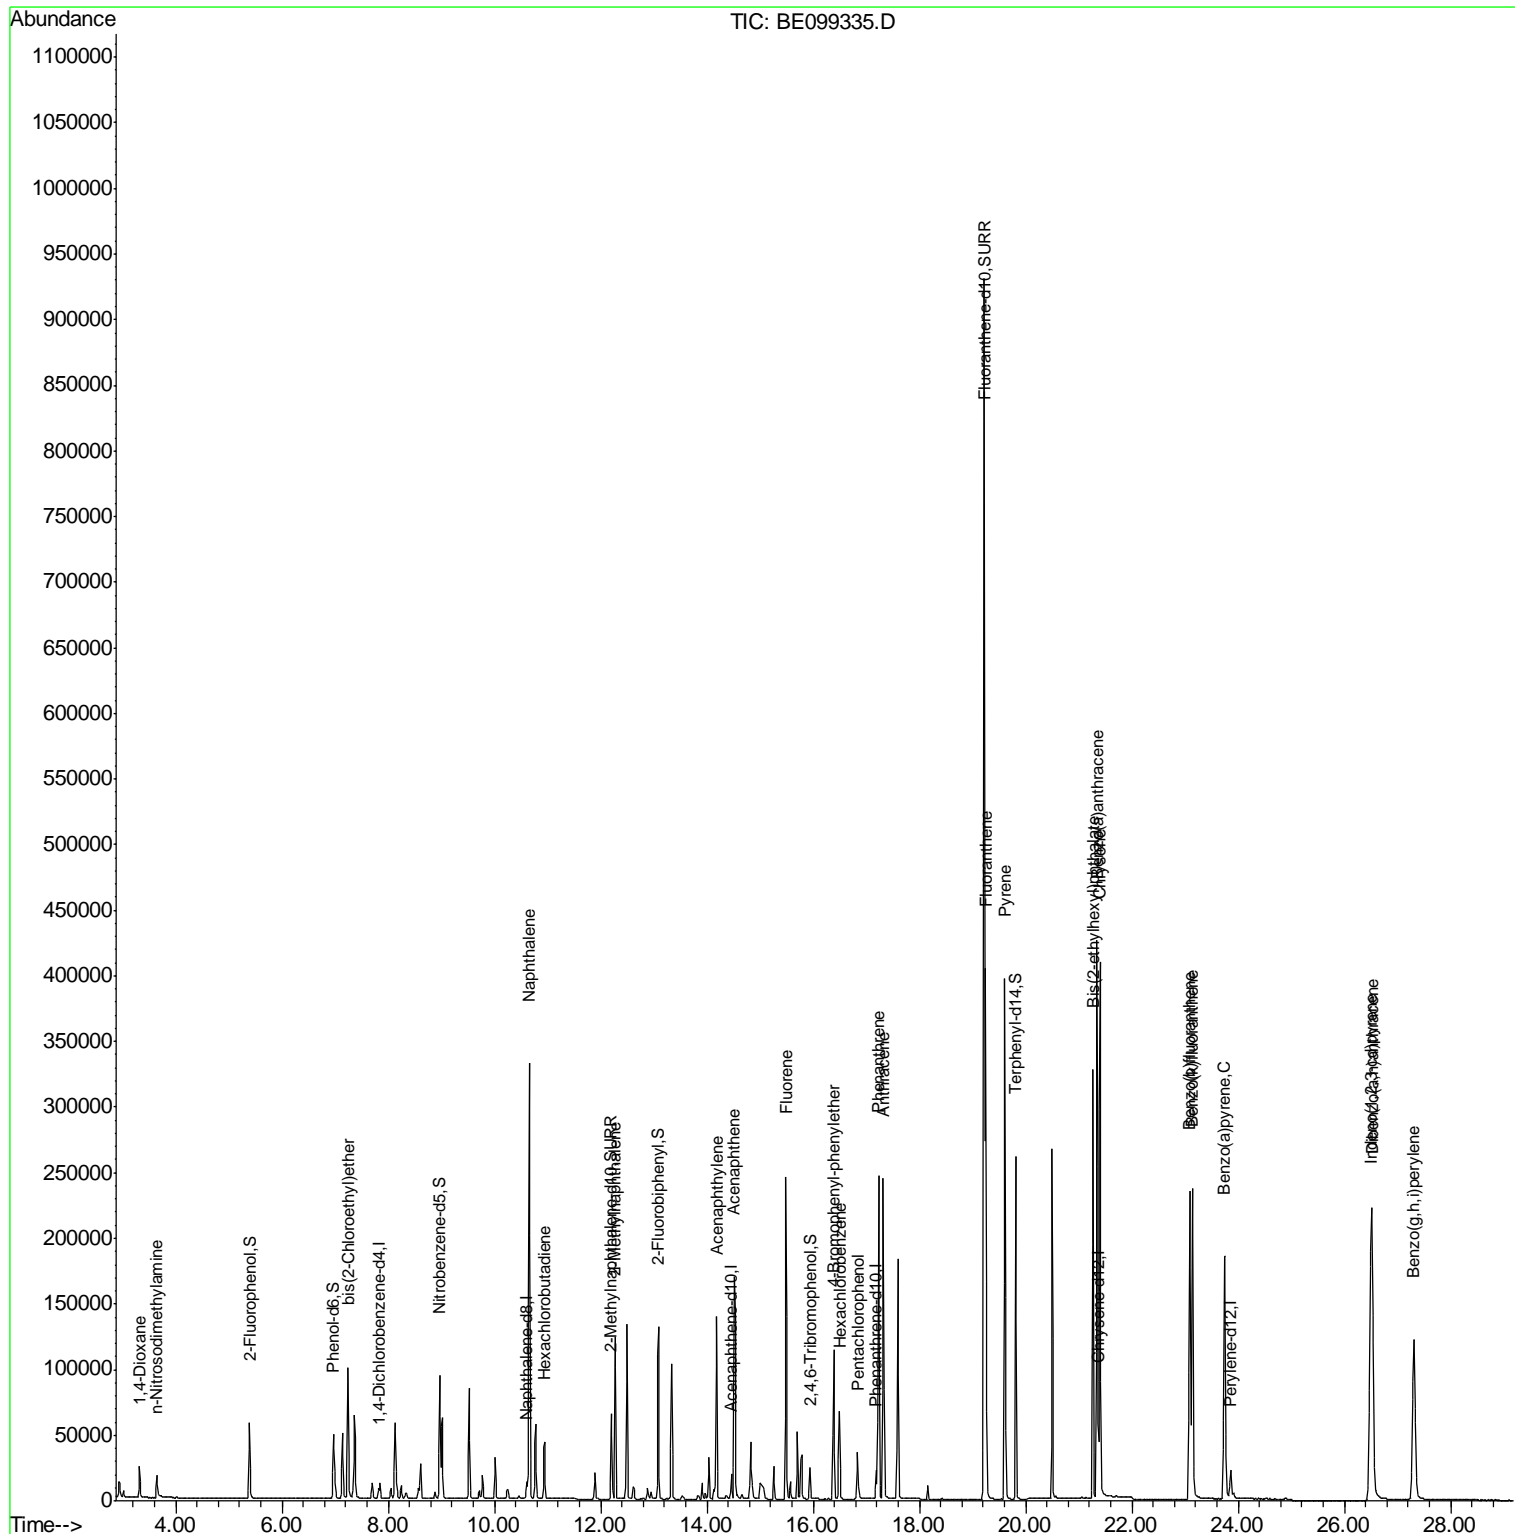




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.82 min Scan# 430
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20




Instrument :
 BNA_E
 ClientSampleID :
 SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
152	3929		
150	100	119.5	179.3
115	144.4	47.5	71.3

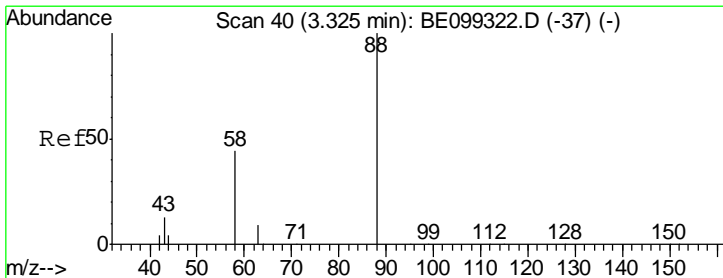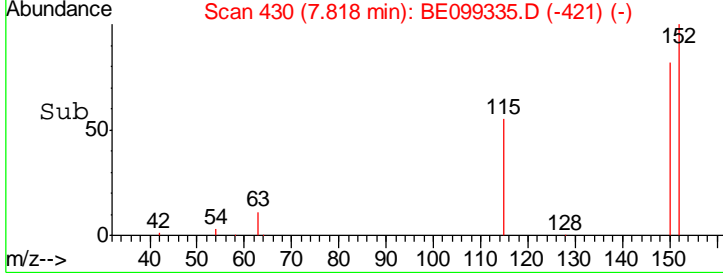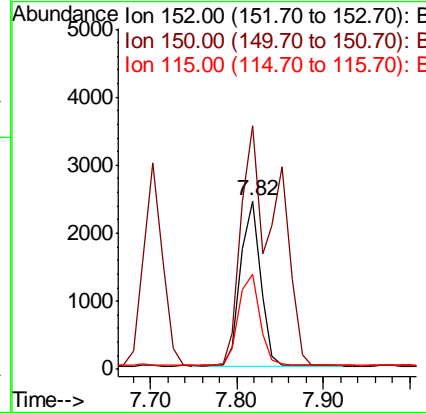

#2
 1,4-Dioxane
 Concen: 3.134 ng
 RT: 3.31 min Scan# 39
 Delta R.T. -0.01 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
88	16777		
58	100	49.1	73.7
43	60.3	17.9	26.9








#3
 n-Nitrosodimethylamine
 Concen: 3.527 ng
 RT: 3.64 min Scan# 67
 Delta R.T. -0.02 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20





Instrument :
 BNA_E
 ClientSampled :
 SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
42	11147		
74	176.3	145.8	218.8
44	6.2	9.0	13.4#

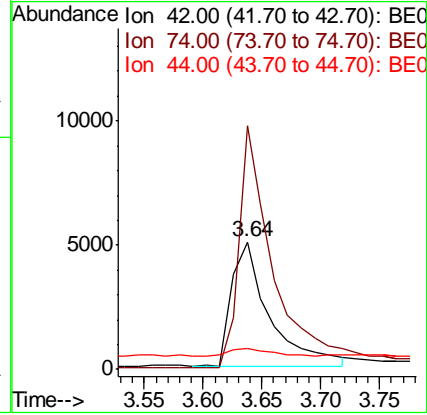

#4
 2-Fluorophenol
 Concen: 2.965 ng
 RT: 5.39 min Scan# 219
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
112	30958		
64	57.0	44.9	67.3
63	120.8	97.4	146.0



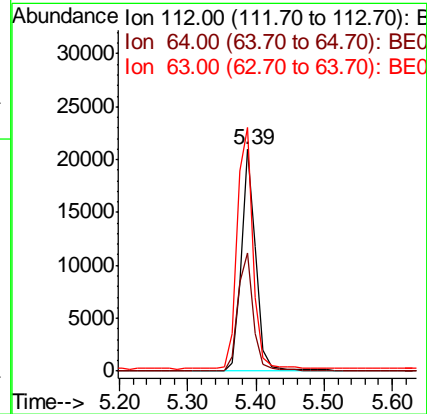





#5
 Phenol-d6
 Concen: 3.167 ng
 RT: 6.97 min Scan# 356
 Delta R.T. -0.01 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20




Instrument :
 BNA_E
ClientSampled :
 SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
99	45462		
42	14.7	11.7	17.5
71	37.2	29.6	44.4

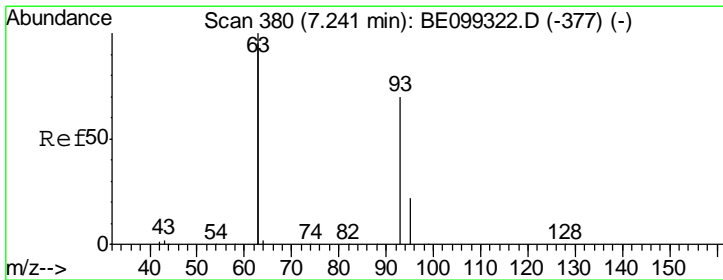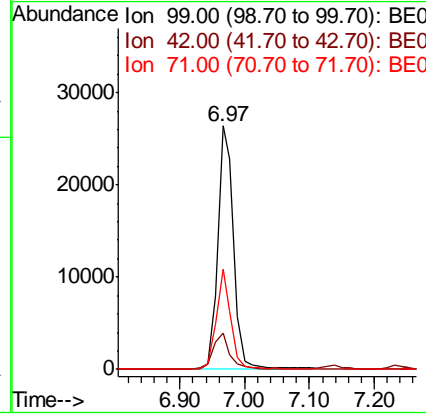

#6
 bis(2-Chloroethyl)ether
 Concen: 3.201 ng
 RT: 7.24 min Scan# 380
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
93	41200		
63	279.4	216.6	324.8
95	32.5	25.8	38.6




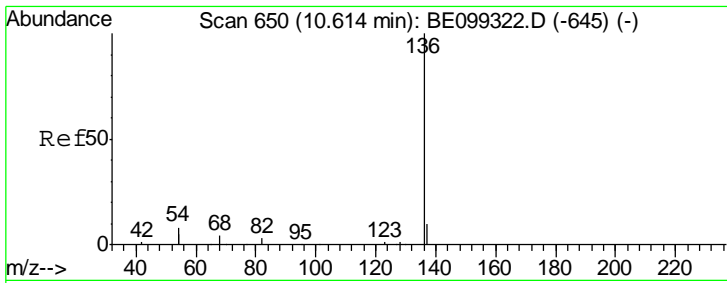




#7
 Naphthalene-d8
 Concen: 0.400 ng
 RT: 10.60 min Scan# 649
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Instrument :
 BNA_E
ClientSampled :
 SSTDICC3.2

Tgt Ion	Resp	Lower	Upper
136	14930		
137	11.1	8.7	13.1
54	30.0	23.8	35.8
68	7.6	6.4	9.6




Abundance
 Ion 136.00 (135.70 to 136.70): E
 Ion 137.00 (136.70 to 137.70): E
 Ion 54.00 (53.70 to 54.70): BE0
 Ion 68.00 (67.70 to 68.70): BE0

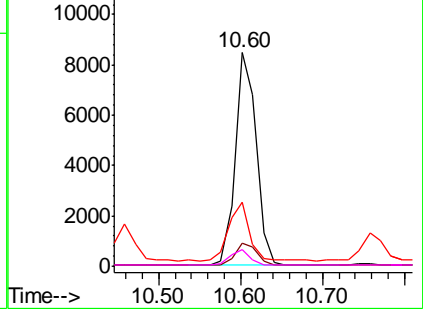
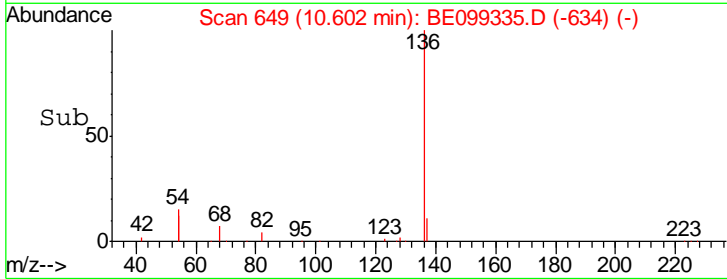



#8
 Nitrobenzene-d5
 Concen: 3.963 ng
 RT: 8.96 min Scan# 523
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
82	40623		
128	111.6	91.7	137.5
54	145.6	122.8	184.2



Abundance
 Ion 82.00 (81.70 to 82.70): BE0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BE0



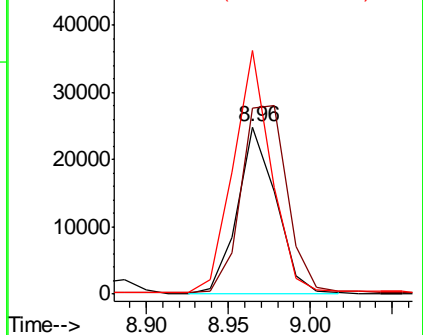
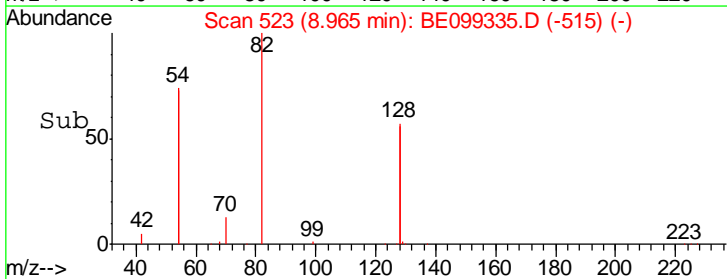


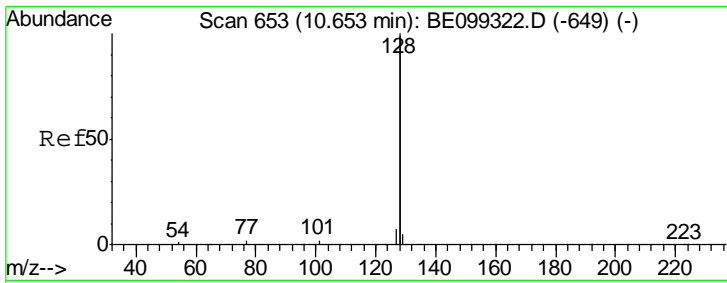

#9
 Naphthalene
 Concen: 3.232 ng
 RT: 10.65 min Scan# 653
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20




Instrument :
 BNA_E
 ClientSampled :
 SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
128	524817		
129	2.8	2.3	3.5
127	3.3	2.8	4.2

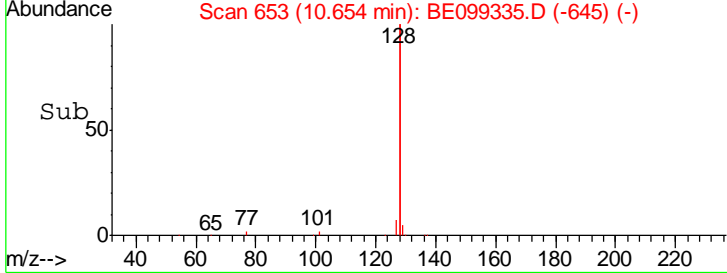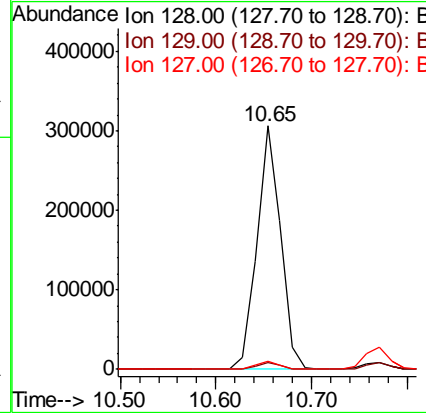

#10
 Hexachlorobutadiene
 Concen: 3.174 ng
 RT: 10.94 min Scan# 675
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
225	33490		
223	62.9	50.3	75.5
227	63.5	49.4	74.0


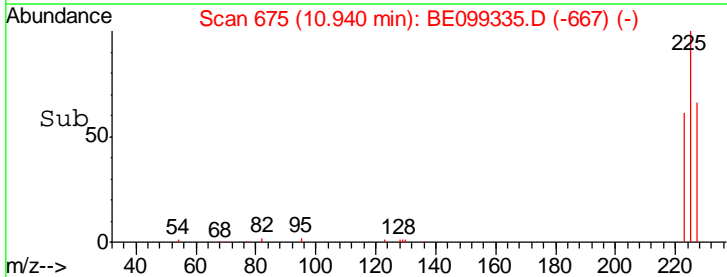






#11
 2-Methylnaphthalene-d10
 Concen: 3.340 ng
 RT: 12.20 min Scan# 762
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20




Instrument :
 BNA_E
 ClientSampleId :
 SSTDIC3.2


Tgt Ion	Resp	Lower	Upper
152	100		
151	19.0	14.9	22.3

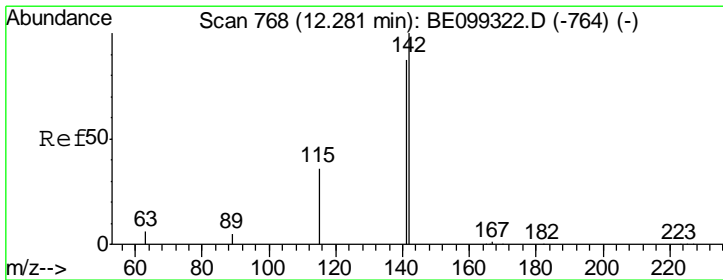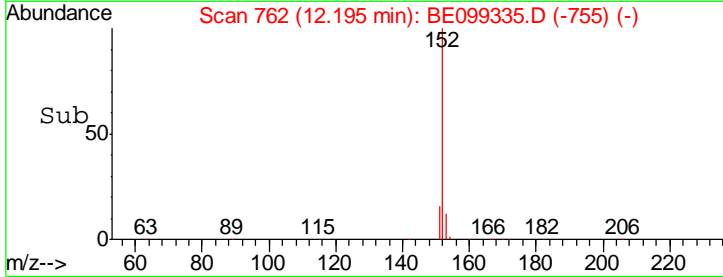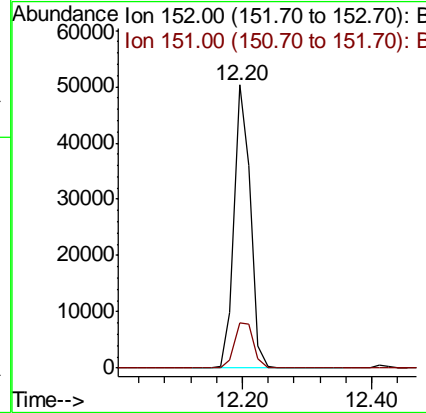

#12
 2-Methylnaphthalene
 Concen: 3.355 ng
 RT: 12.27 min Scan# 767
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
142	100		
141	91.8	72.0	108.0
115	39.8	33.4	50.0


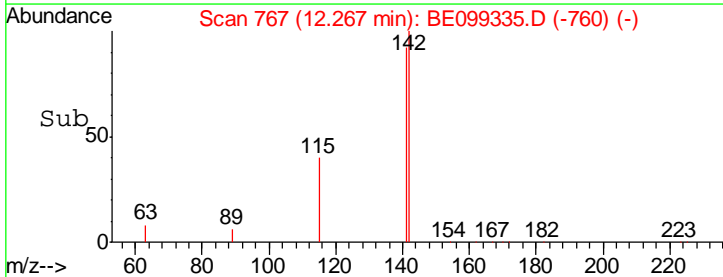

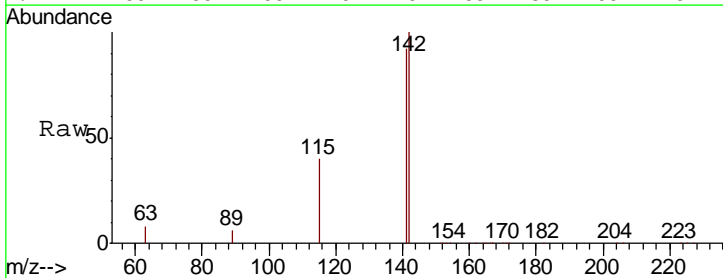


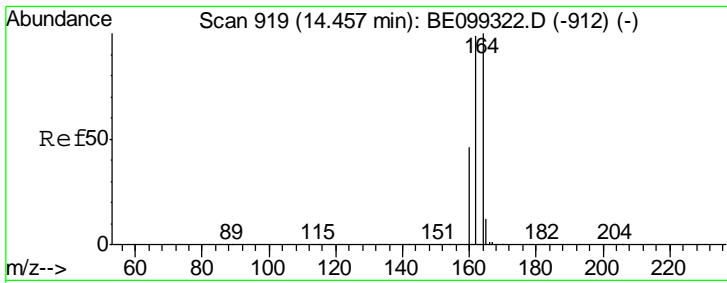

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.46 min Scan# 919
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20




Instrument :
 BNA_E
ClientSampled :
 SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
164	10580		
162	98.5	77.8	116.6
160	46.8	37.1	55.7

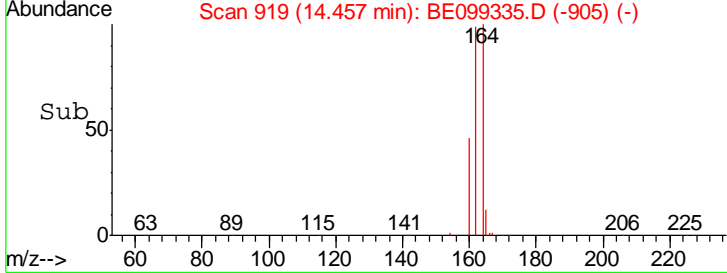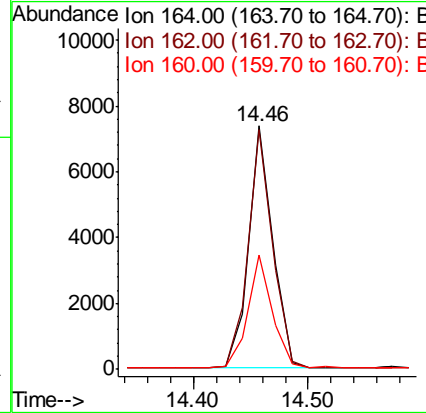

#14
 2,4,6-Tribromophenol
 Concen: 3.310 ng
 RT: 15.94 min Scan# 1024
 Delta R.T. -0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
330	16136		
332	97.4	82.5	123.7
141	32.5	24.9	37.3


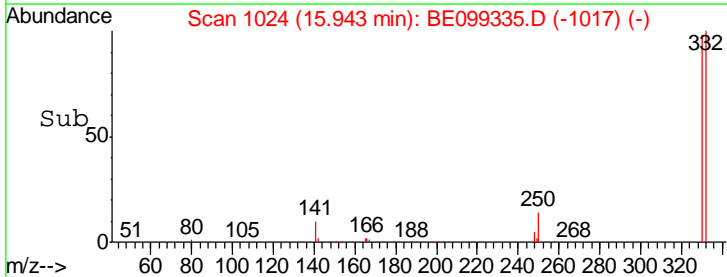




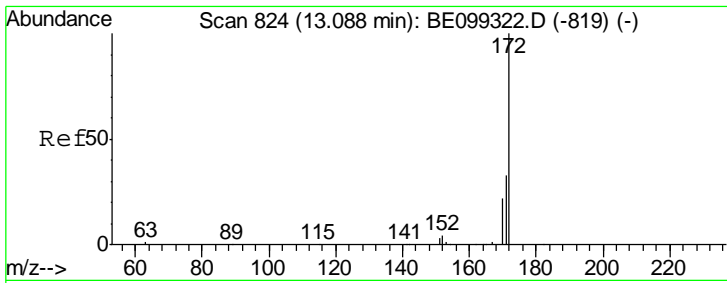

#15
 2-Fluorobiphenyl
 Concen: 3.212 ng
 RT: 13.09 min Scan# 824
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20




Instrument :
 BNA_E
 ClientSampled :
 SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
172	133592		
171	33.6	26.2	39.2
170	22.0	18.1	27.1

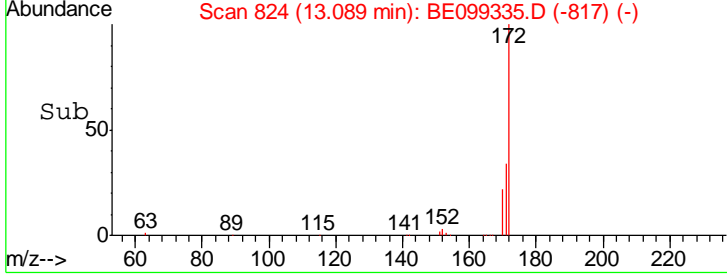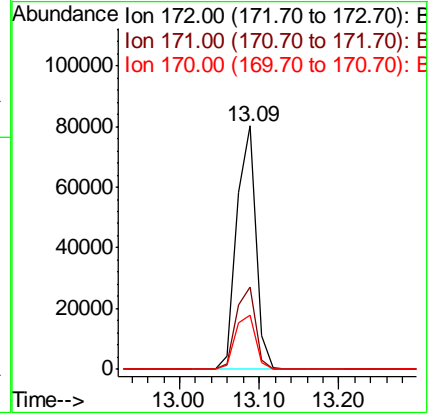

#16
 Acenaphthylene
 Concen: 3.401 ng
 RT: 14.18 min Scan# 900
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
152	170479		
151	19.7	15.5	23.3
153	13.1	10.2	15.4

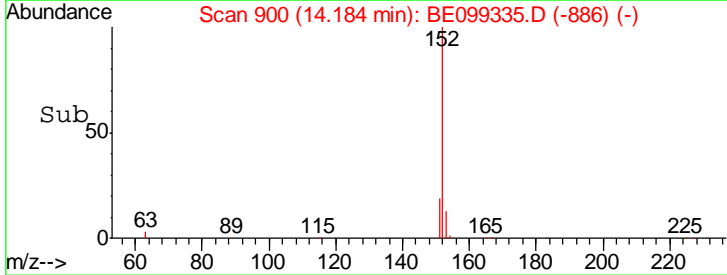
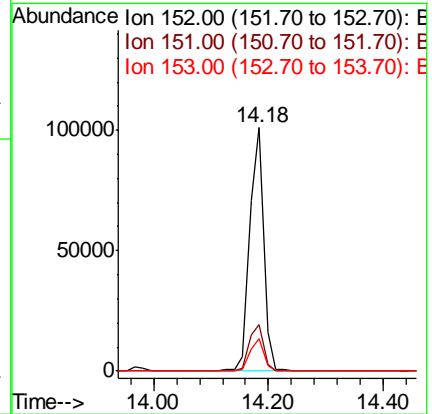



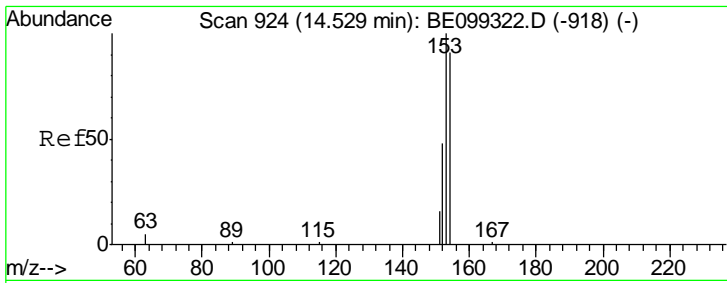

#17
 Acenaphthene
 Concen: 3.292 ng
 RT: 14.51 min Scan# 923
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20





Instrument :
 BNA_E
ClientSampled :
 SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
154	100		
153	115.6	94.7	142.1
152	56.2	46.4	69.6

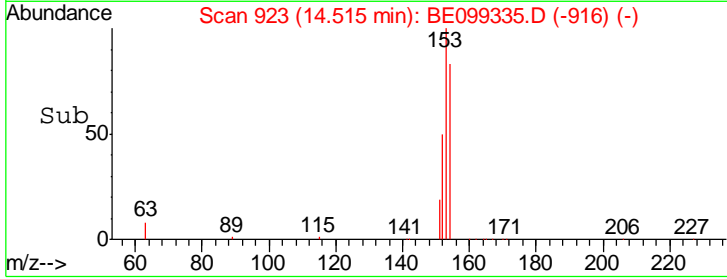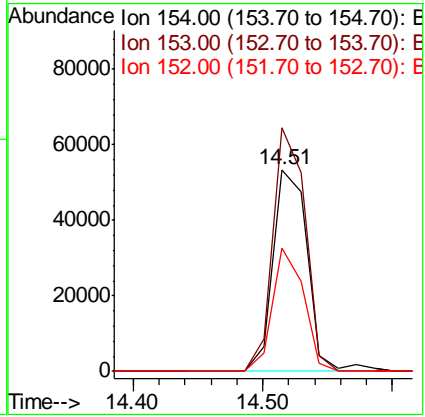

#18
 Fluorene
 Concen: 3.275 ng
 RT: 15.49 min Scan# 990
 Delta R.T. -0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
166	100		
165	100.3	79.7	119.5
167	13.4	11.0	16.4

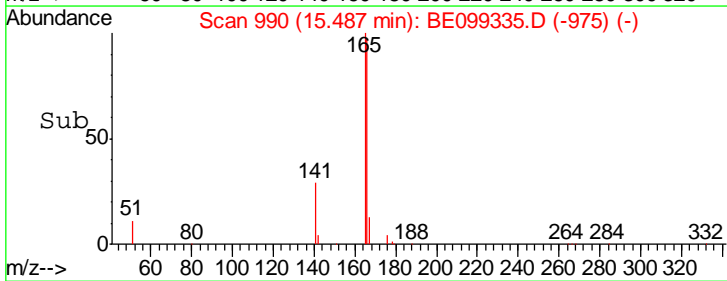
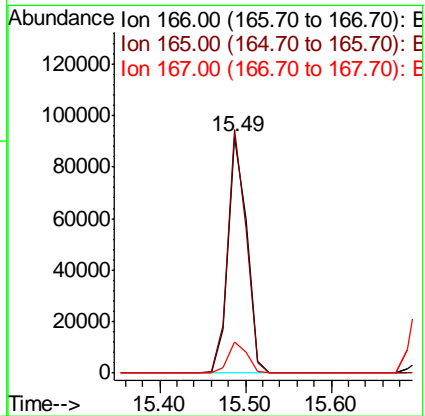



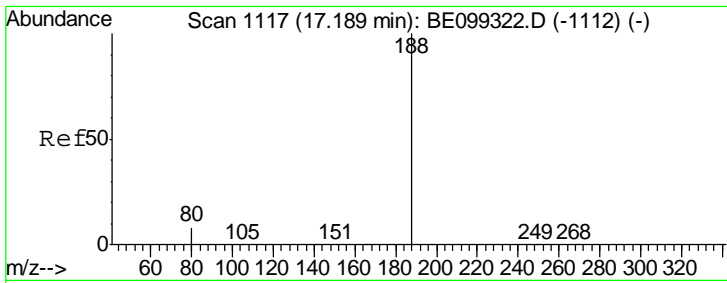

#19
 Phenanthrene-d10
 Concen: 0.400 ng
 RT: 17.19 min Scan# 1117
 Delta R.T. -0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20





Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
188	29303		
94	0.0	0.0	0.0
80	7.7	6.2	9.4

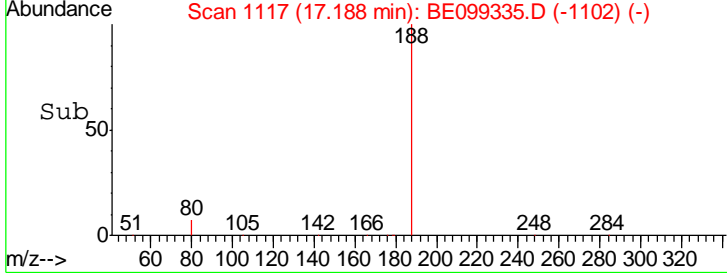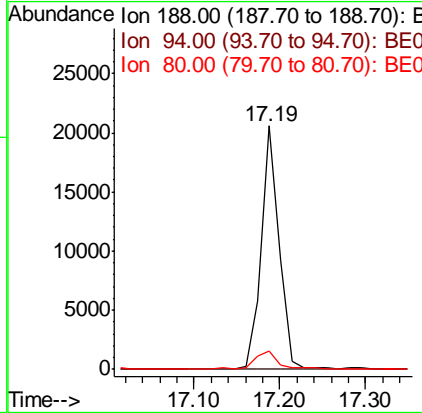

#20
 4-Bromophenyl-phenylether
 Concen: 3.344 ng
 RT: 16.38 min Scan# 1057
 Delta R.T. -0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
248	55625		
250	93.3	77.0	115.6
141	43.4	31.1	46.7

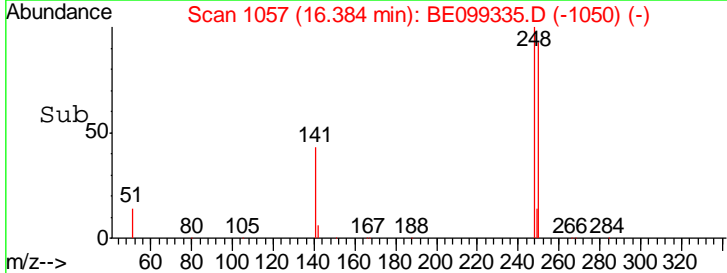

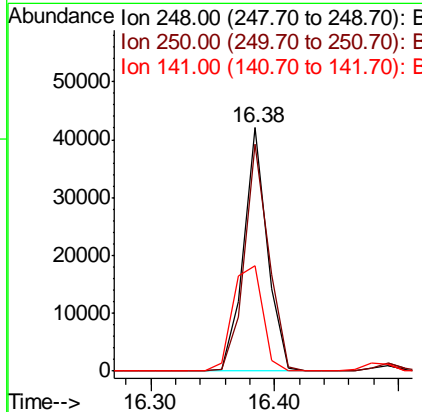
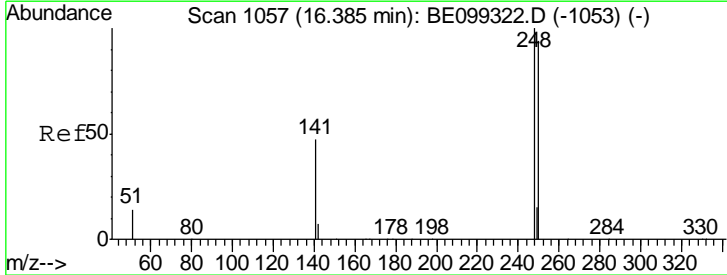


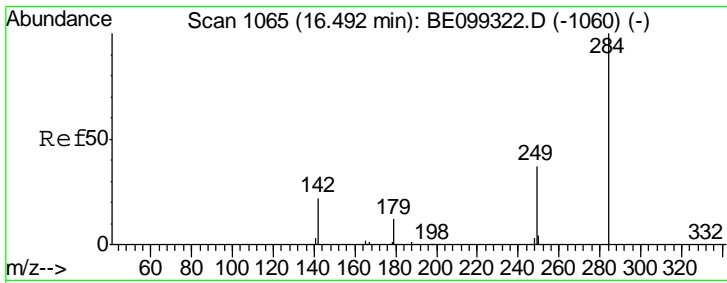

#21
 Hexachlorobenzene
 Concen: 3.326 ng
 RT: 16.49 min Scan# 1065
 Delta R.T. -0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20




Instrument :
 BNA_E
 ClientSampleId :
 SSTDIC3.2


Tgt Ion	Resp	Lower	Upper
284	52668		
142	28.2	21.8	32.6
249	33.3	26.2	39.4

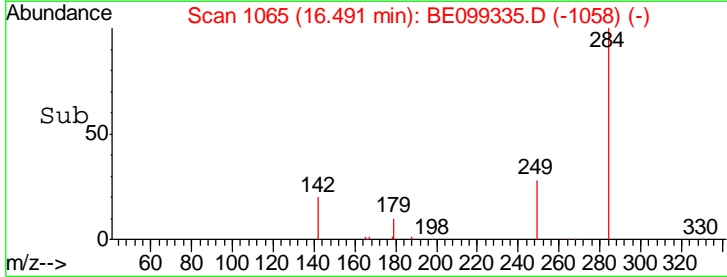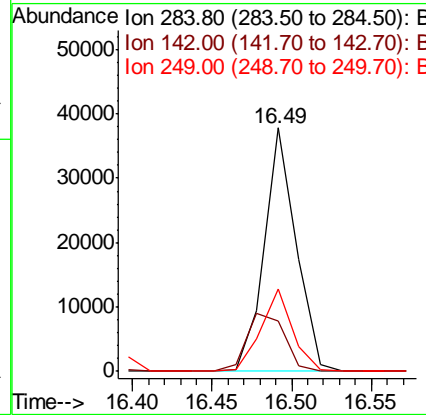

#22
 Pentachlorophenol
 Concen: 2.941 ng
 RT: 16.84 min Scan# 1091
 Delta R.T. -0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
266	19339		
264	62.5	54.5	81.7
268	64.8	54.3	81.5

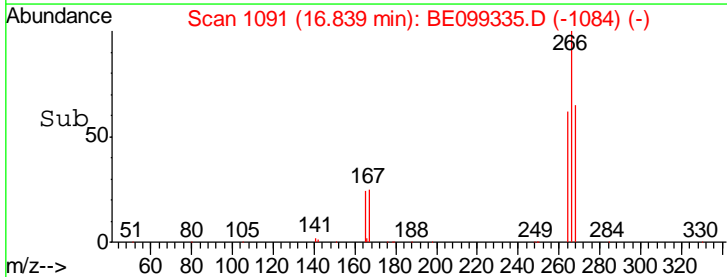




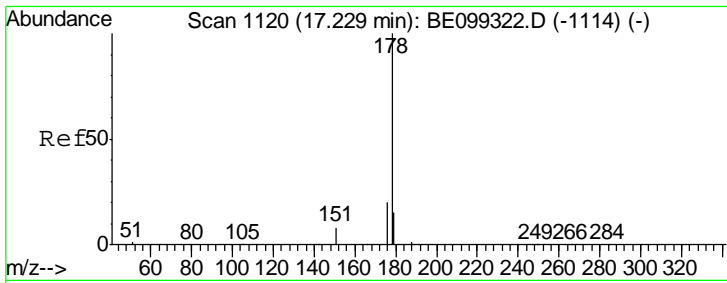

#23
 Phenanthrene
 Concen: 3.333 ng
 RT: 17.23 min Scan# 1120
 Delta R.T. -0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20





Instrument :
 BNA_E
 ClientSampled :
 SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
178	252752		
176	19.5	15.3	22.9
179	15.5	12.4	18.6

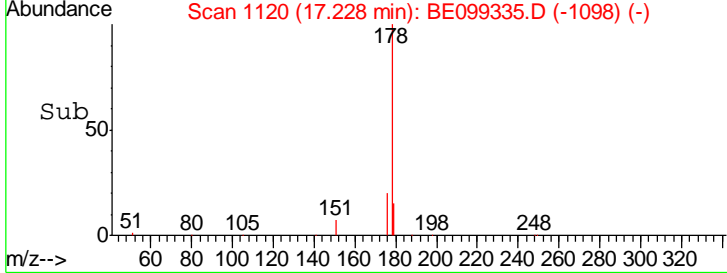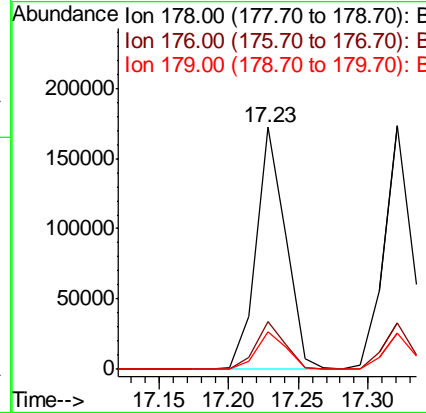

#24
 Anthracene
 Concen: 3.347 ng
 RT: 17.32 min Scan# 1127
 Delta R.T. -0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
178	239374		
176	19.0	15.1	22.7
179	15.3	11.9	17.9

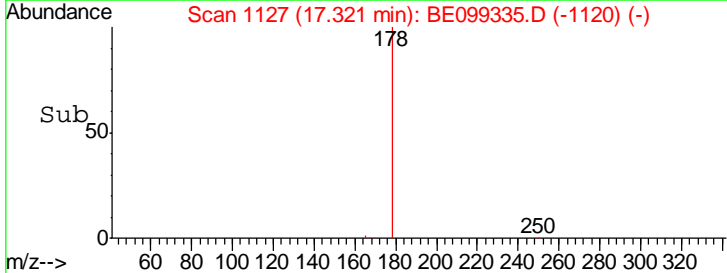

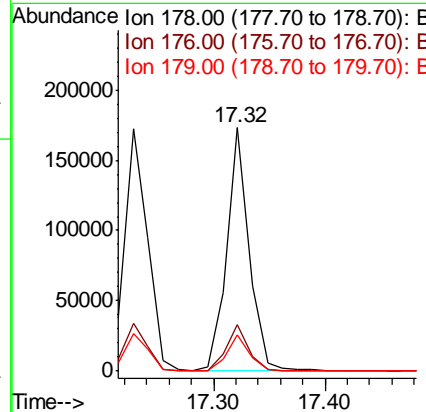
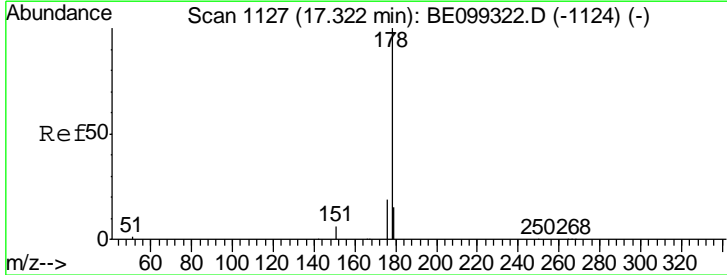




#25
 Fluoranthene-d10
 Concen: 3.087 ng
 RT: 19.22 min Scan# 1384
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
212	1193886		
106	2.2	1.8	2.6
104	1.2	1.0	1.4

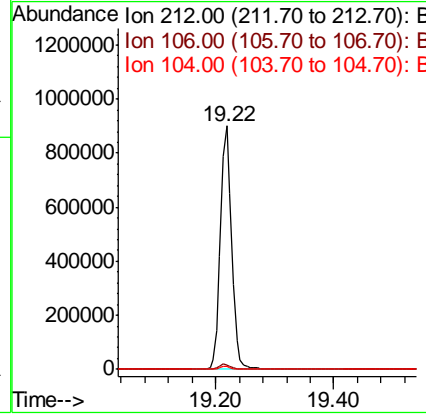

#26
 Fluoranthene
 Concen: 3.196 ng
 RT: 19.25 min Scan# 1389
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
202	357678		
101	7.8	6.4	9.6
203	17.4	13.5	20.3


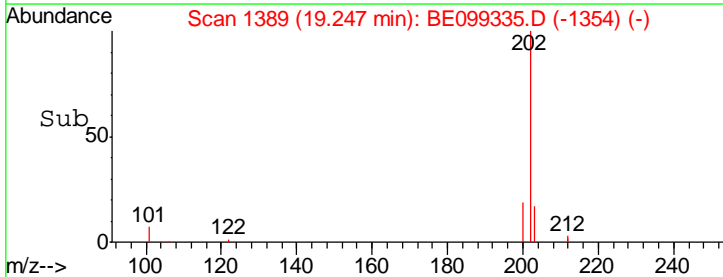






#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.37 min Scan# 1630
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20




Instrument :
 BNA_E
 ClientSampled :
 SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
240	37224		
120	2.7	2.2	3.2
236	25.5	20.2	30.4

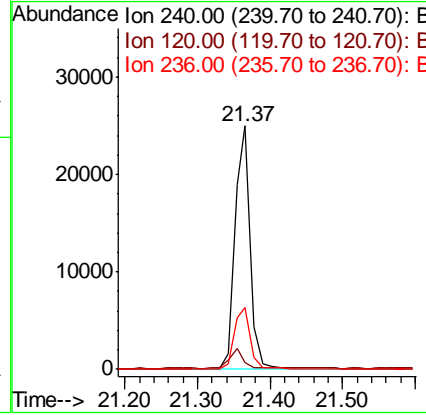

#28
 Pyrene
 Concen: 3.632 ng
 RT: 19.61 min Scan# 1452
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
202	357087		
200	19.8	15.7	23.5
203	17.7	13.7	20.5









#29
 Terphenyl-d14
 Concen: 3.524 ng
 RT: 19.82 min Scan# 1488
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20




Instrument : BNA_E
 ClientSampled : SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
244	239302		
212	29.0	22.6	33.8
122	5.7	4.6	7.0

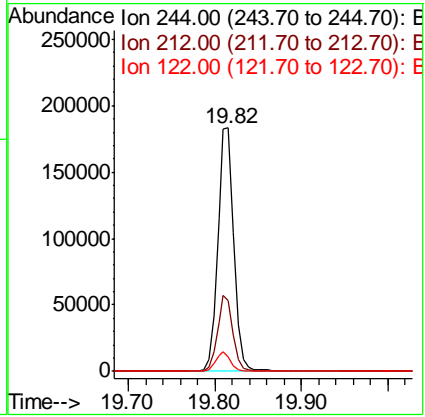

#30
 Benzo(a)anthracene
 Concen: 3.122 ng
 RT: 21.34 min Scan# 1628
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
228	365841		
226	27.9	22.0	33.0
229	19.4	15.8	23.8


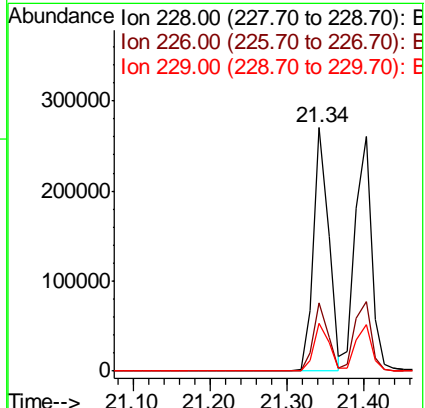






#31
 Chrysene
 Concen: 3.322 ng
 RT: 21.40 min Scan# 1633
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20




Instrument :
 BNA_E
 ClientSampled :
 SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
228	381784		
226	29.5	23.4	35.2
229	19.9	16.2	24.2

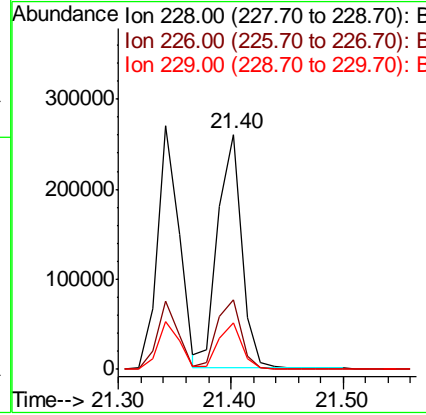

#32
 Bis(2-ethylhexyl)phthalate
 Concen: 2.505 ng
 RT: 21.27 min Scan# 1622
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
149	374295		
167	7.5	6.0	9.0
279	1.2	1.1	1.7


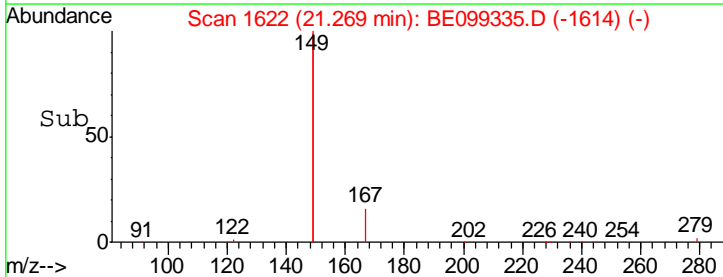






#33
 Indeno(1,2,3-cd)pyrene
 Concen: 2.889 ng
 RT: 26.49 min Scan# 2932
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20




Instrument :
 BNA_E
 ClientSampled :
 SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
276	379461		
138	15.4	12.7	19.1
277	24.7	19.6	29.4

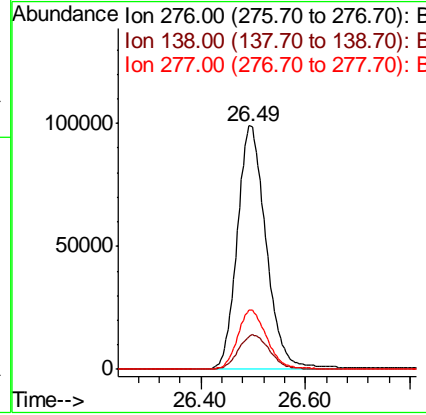

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.86 min Scan# 2196
 Delta R.T. -0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
264	32616		
260	24.4	20.1	30.1
265	24.7	19.9	29.9

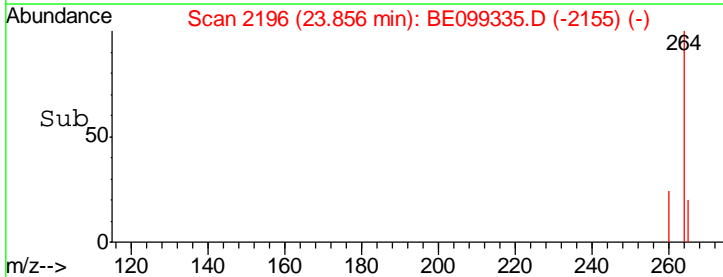






#35
 Benzo(b)fluoranthene
 Concen: 3.486 ng
 RT: 23.09 min Scan# 1980
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20





Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
252	339246		
253	21.7	17.3	25.9
125	6.3	5.8	8.6

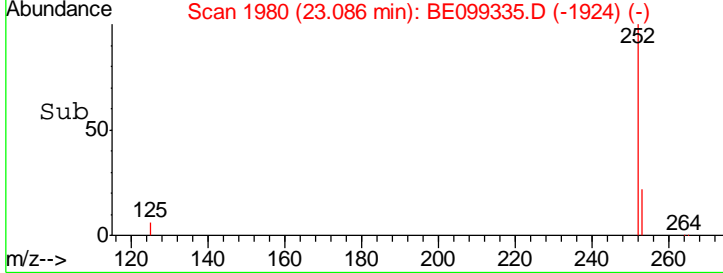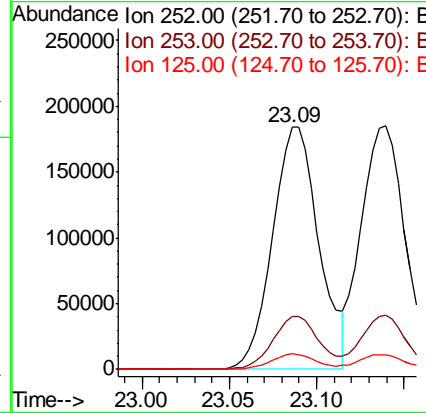

#36
 Benzo(k)fluoranthene
 Concen: 3.552 ng
 RT: 23.14 min Scan# 1995
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
252	336406		
253	22.1	18.4	27.6
125	6.1	5.4	8.0

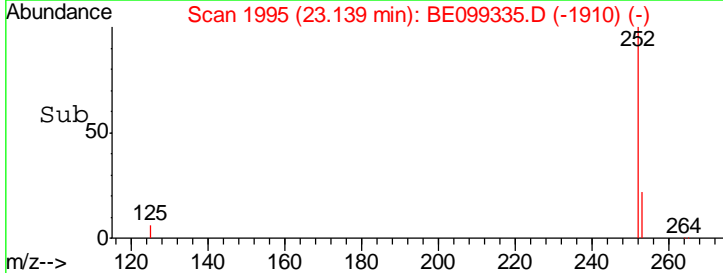

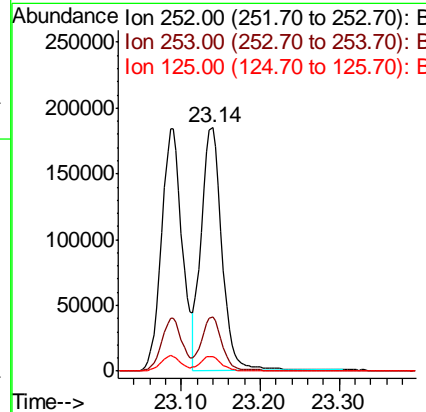





#37
 Benzo(a)pyrene
 Concen: 3.355 ng
 RT: 23.74 min Scan# 2164
 Delta R.T. -0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20




Instrument :
 BNA_E
 ClientSampled :
 SSTDICC3.2


Tgt Ion	Resp	Lower	Upper
252	306936		
253	22.1	17.6	26.4
125	6.8	6.5	9.7

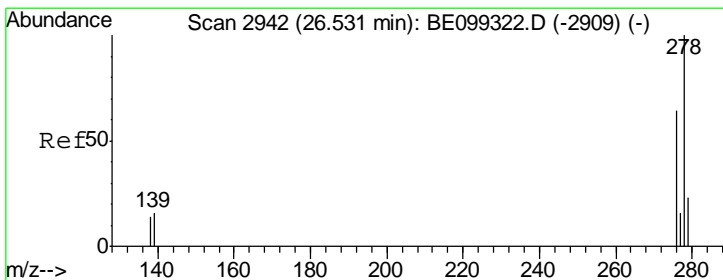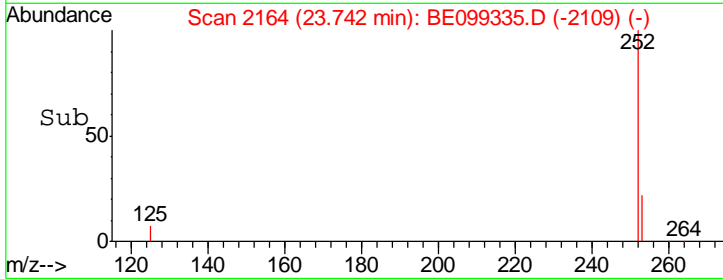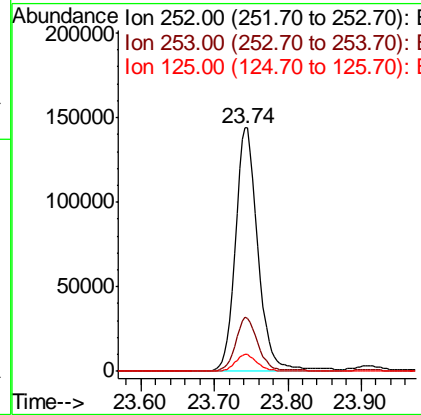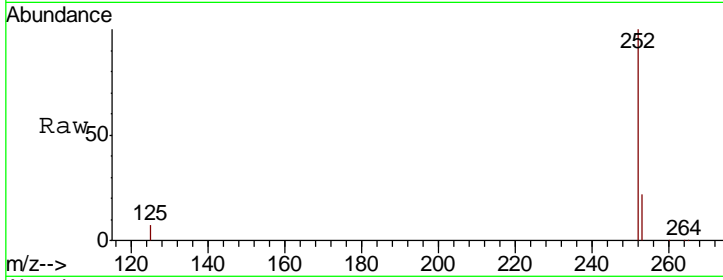

#38
 Dibenzo(a,h)anthracene
 Concen: 3.472 ng
 RT: 26.52 min Scan# 2940
 Delta R.T. 0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Tgt Ion	Resp	Lower	Upper
278	315852		
139	9.9	8.5	12.7
279	23.6	19.8	29.8

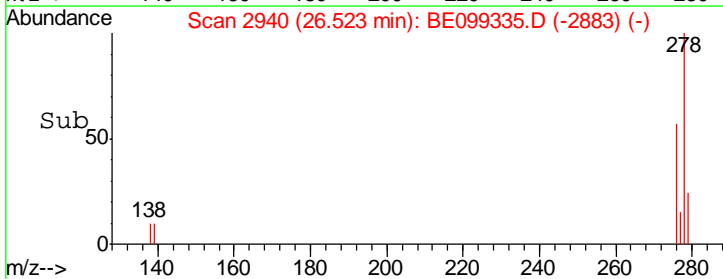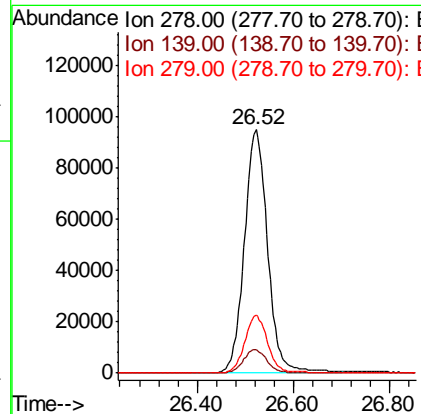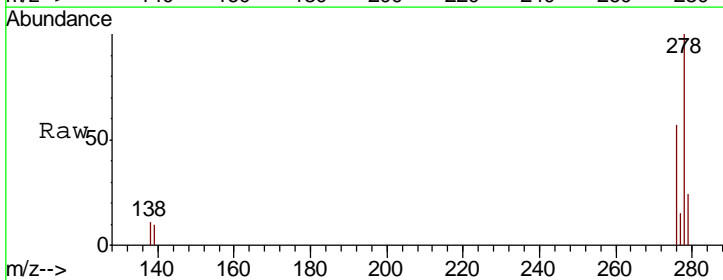



#39
 Benzo(a,h,i)perylene
 Concen: 3.463 ng
 RT: 27.30 min Scan# 3159
 Delta R.T. -0.00 min
 Lab File: BE099335.D
 Acq: 18 Apr 2019 12:20

Instrument :
 BNA_E
 ClientSampled :
 SSTDICC3.2

Tot Ion	Resp	Lower	Upper
276	100		
277	24.0	20.0	30.0
138	13.5	11.1	16.7

