
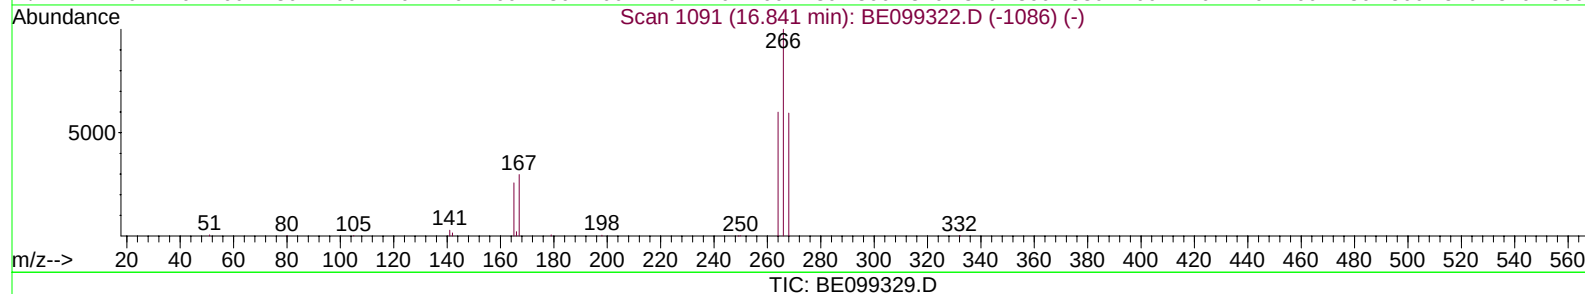
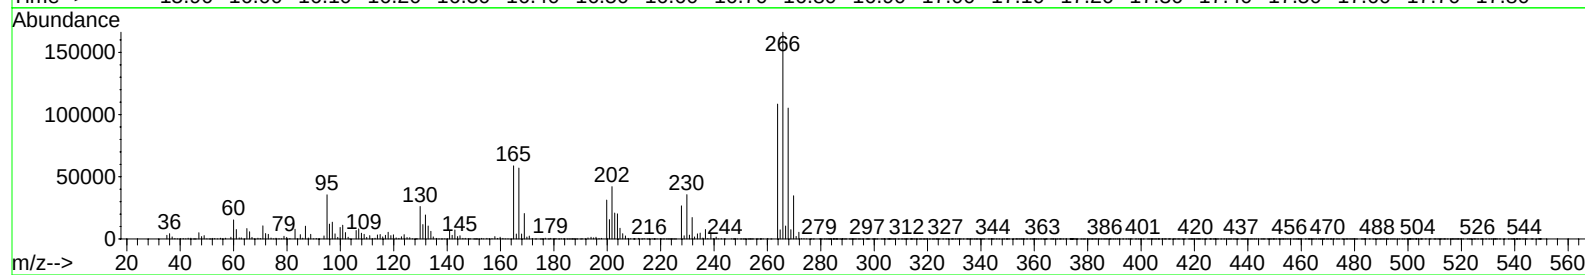


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE041819\
Data File : BE099329.D
Acq On : 18 Apr 2019 8:36
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 18 17:54:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE041819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 18 14:50:20 2019
Response via : Initial Calibration

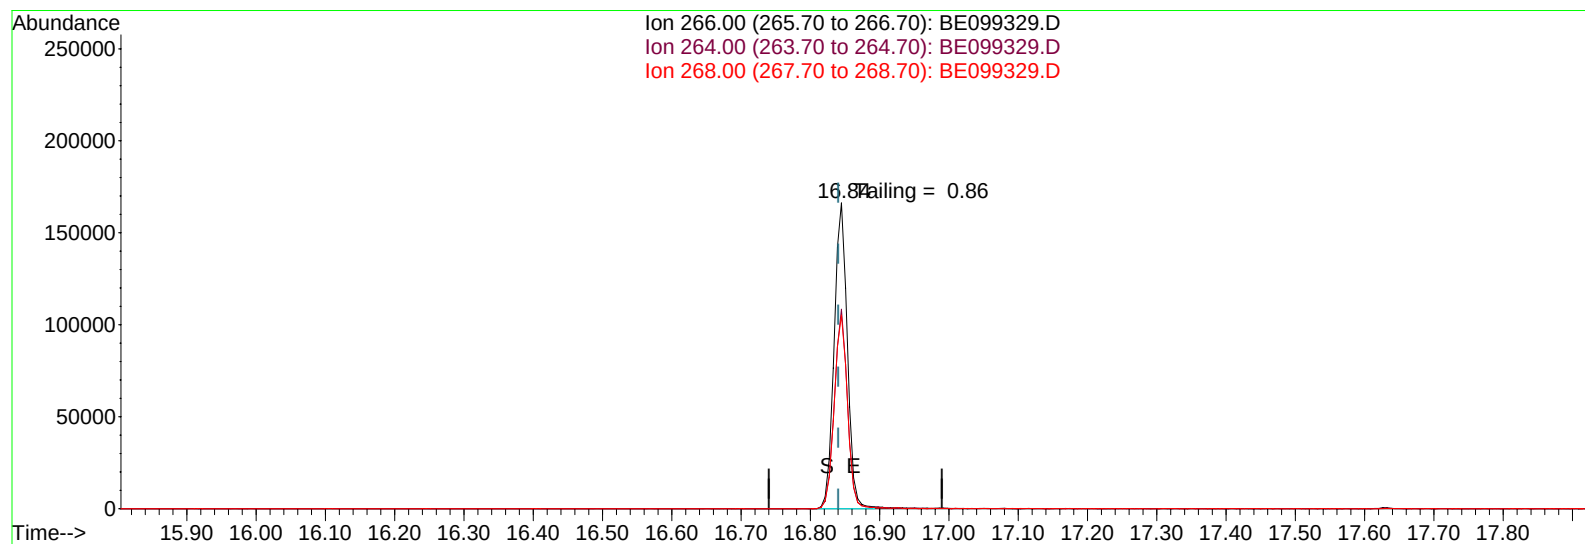

(22) Pentachlorophenol

16.845min (+0.005) 3189.09ng

response 220814

Ion	Exp%	Act%
266.00	100	100
264.00	68.10	65.28
268.00	67.90	63.34
0.00	0.00	0.00