


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE041819\
Data File : BE099329.D
Acq On : 18 Apr 2019 8:36
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041819.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 19 06:51:38 2019

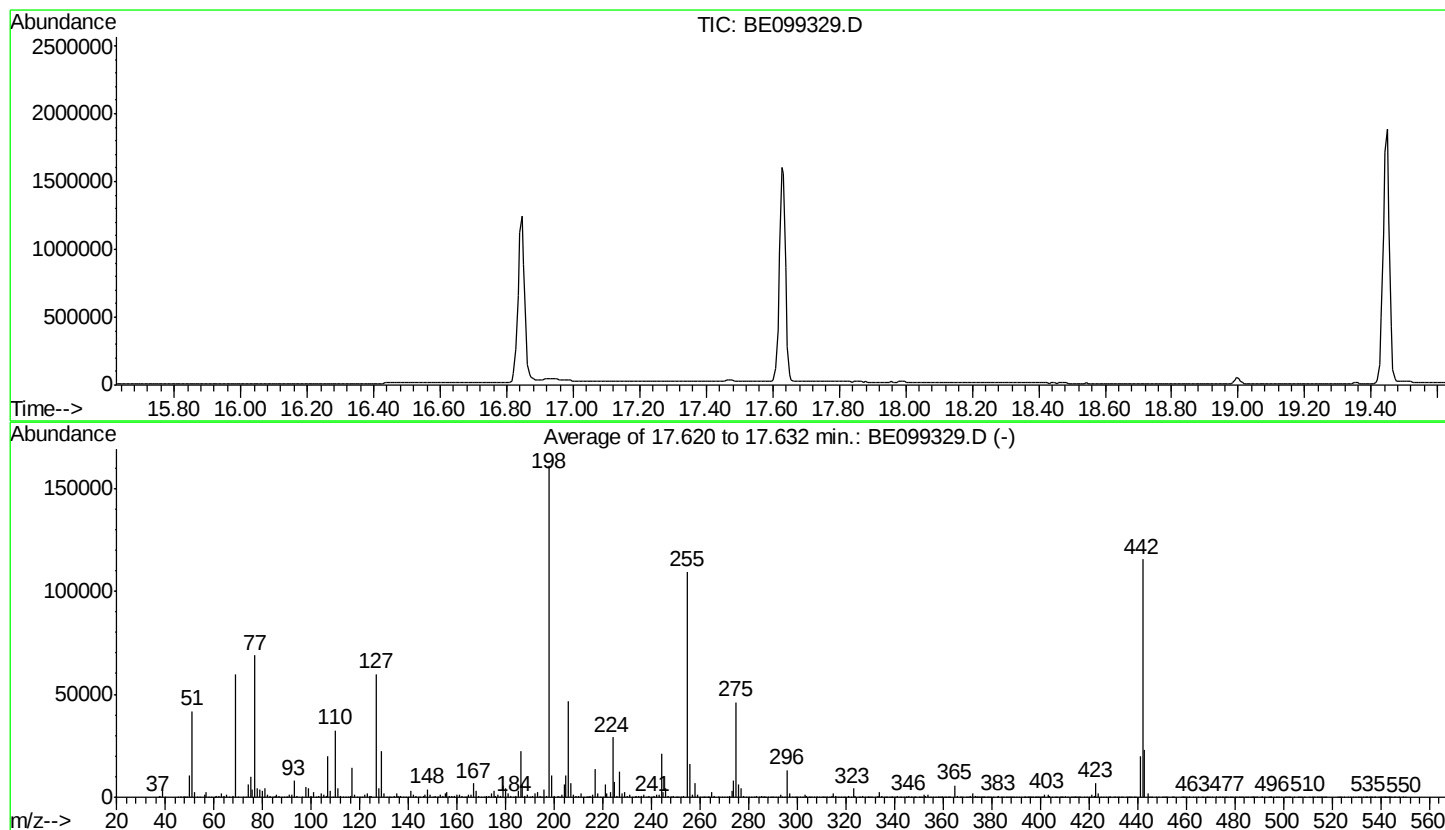

AutoFind: Scans 2558, 2559, 2560; Background Corrected with Scan 2551

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.9	41644	PASS
68	69	0.00	2	0.9	533	PASS
69	198	0.00	100	37.0	59622	PASS
70	69	0.00	2	0.3	193	PASS
127	198	10	80	37.1	59774	PASS
197	198	0.00	2	0.2	387	PASS
198	198	100	100	100.0	160964	PASS
199	198	5	9	6.5	10487	PASS
275	198	10	60	28.6	46026	PASS
365	198	1	100	3.6	5858	PASS
441	198	0.01	100	12.4	19974	PASS
442	198	50	100	71.7	115431	PASS
443	442	15	24	19.8	22877	PASS