


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE041919\
 Data File : BE099345.D
 Acq On : 19 Apr 2019 12:37
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 19 06:51:38 2019

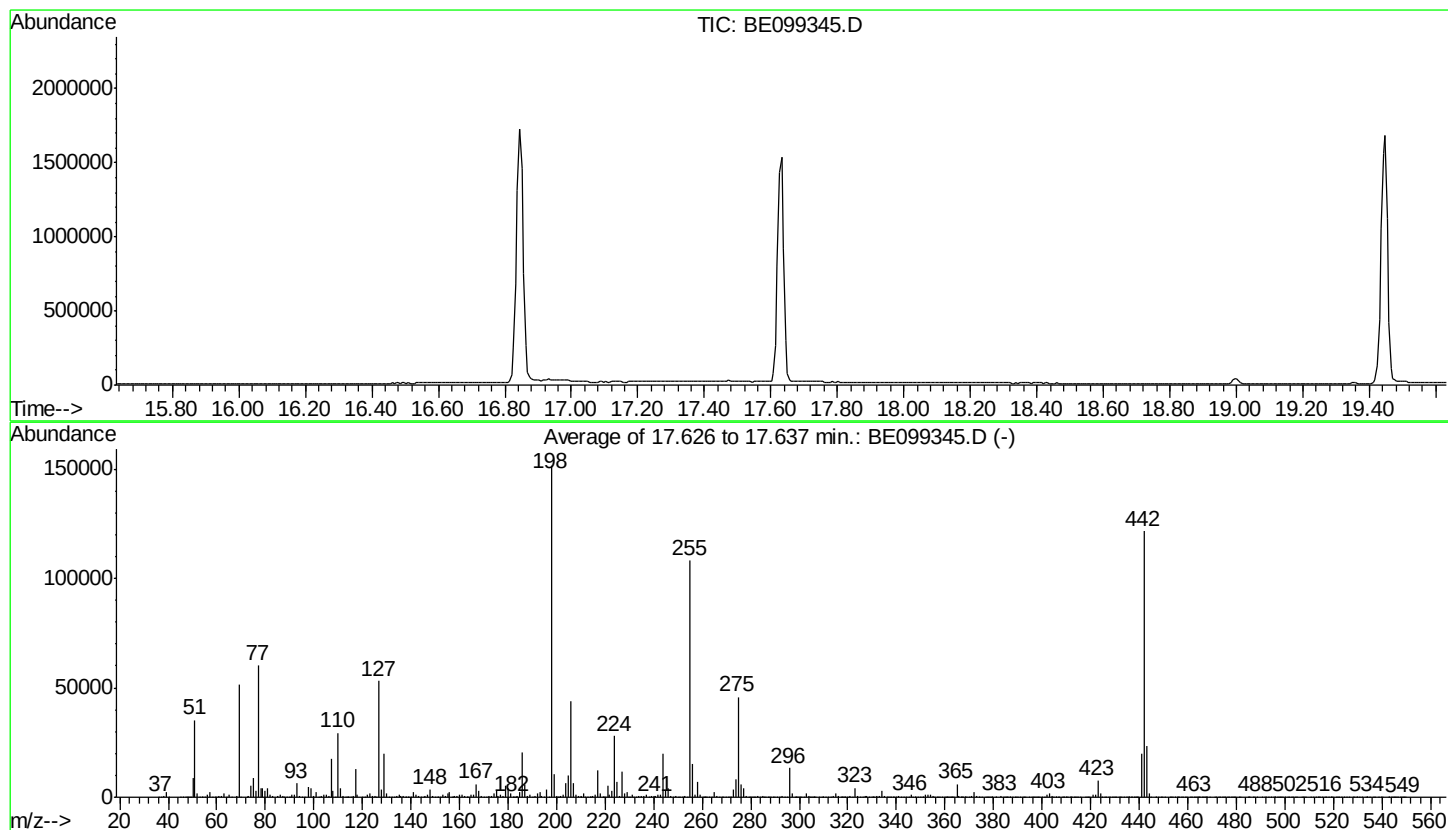

AutoFind: Scans 2559, 2560, 2561; Background Corrected with Scan 2551

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.3	35289	PASS
68	69	0.00	2	1.6	842	PASS
69	198	0.00	100	33.9	51323	PASS
70	69	0.00	2	0.6	286	PASS
127	198	10	80	35.0	53002	PASS
197	198	0.00	2	0.1	154	PASS
198	198	100	100	100.0	151481	PASS
199	198	5	9	7.0	10531	PASS
275	198	10	60	30.2	45818	PASS
365	198	1	100	3.9	5883	PASS
441	198	0.01	100	13.3	20104	PASS
442	198	50	100	80.2	121535	PASS
443	442	15	24	19.3	23504	PASS