

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE042619\
 Data File : BE099385.D
 Acq On : 26 Apr 2019 19:19
 Operator : JU/SJ
 Sample : K2569-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PST-003-SW024-042319

Manual Integrations
 APPROVED

Sohil
 4/29/2019 1:28:50 PM

Quant Time: Apr 27 06:50:35 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE041819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Apr 19 06:51:38 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	4182	0.40	ng	0.00
7) Naphthalene-d8	10.61	136	16136	0.40	ng	0.01
13) Acenaphthene-d10	14.46	164	10969	0.40	ng	0.00
19) Phenanthrene-d10	17.19	188	29241	0.40	ng	0.00
27) Chrysene-d12	21.37	240	32236	0.40	ng	0.00
34) Perylene-d12	23.87	264	37094	0.40	ng	0.01

System Monitoring Compounds

4) 2-Fluorophenol	5.40	112	3178	0.31	ng	0.01
5) Phenol-d6	6.98	99	4923	0.34	ng	0.00
8) Nitrobenzene-d5	8.98	82	4081	0.33	ng	0.01
11) 2-Methylnaphthalene-d10	12.21	152	7503	0.26	ng	0.01
14) 2,4,6-Tribromophenol	15.94	330	1712	0.47	ng	0.00
15) 2-Fluorobiphenyl	13.09	172	11080	0.26	ng	0.00
25) Fluoranthene-d10	19.22	212	88416	0.25	ng	0.00
29) Terphenyl-d14	19.82	244	18857	0.30	ng	0.00

Target Compounds

						Qvalue
9) Naphthalene	10.65	128	43797	0.249	ng	100
12) 2-Methylnaphthalene	12.28	142	6253	0.209	ng	97
16) Acenaphthylene	14.18	152	1549	0.031	ng	# 83
17) Acenaphthene	14.53	154	6852	0.224	ng	99
18) Fluorene	15.50	166	7193	0.164	ng	98
23) Phenanthrene	17.24	178	143672	1.855	ng	99
24) Anthracene	17.32	178	20123	0.292	ng	# 90
26) Fluoranthene	19.25	202	187238	1.807	ng	98
28) Pyrene	19.62	202	160477	1.690	ng	# 95
30) Benzo(a)anthracene	21.36	228	95748	1.010	ng	98
31) Chrysene	21.40	228	78340	0.777	ng	96
32) Bis(2-ethylhexyl)phthalate	21.27	149	16482	0.191	ng	# 100
33) Indeno(1,2,3-cd)pyrene	26.52	276	36088	0.362	ng	# 92
35) Benzo(b)fluoranthene	23.10	252	94394	0.831	ng	95
36) Benzo(k)fluoranthene	23.15	252	31132m	0.275	ng	
37) Benzo(a)pyrene	23.75	252	67506	0.663	ng	96
38) Dibenzo(a,h)anthracene	26.54	278	8830	0.085	ng	# 75
39) Benzo(a,h,i)perylene	27.34	276	33048	0.313	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE042619\
Data File : BE099385.D
Acq On : 26 Apr 2019 19:19
Operator : JU/SJ
Sample : K2569-06
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
PST-003-SW024-042319

Manual Integrations
APPROVED

Sohil
4/29/2019 1:28:50 PM

Quant Time: Apr 27 06:50:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE041819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 19 06:51:38 2019
Response via : Initial Calibration





#1


1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.82 min Scan# 430
Delta R.T. -0.00 min
Lab File: BE099385.D
Acq: 26 Apr 2019 19:19

Instrument :
BNA_E
ClientSampleId :
PST-003-SW024-042319

Tot Ion	Ratio	Lower	Upper
152	100		
150	150.5	119.5	179.3
115	61.7	47.5	71.3

Manual Integrations
APPROVED

Sohil
4/29/2019 1:28:50 PM





Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

Time-->



#4

2-Fluorophenol
Concen: 0.311 ng
RT: 5.40 min Scan# 220
Delta R.T. 0.01 min
Lab File: BE099385.D
Acq: 26 Apr 2019 19:19

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.4	44.9	67.3
63	127.1	97.4	146.0



Abundance


Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

Time-->



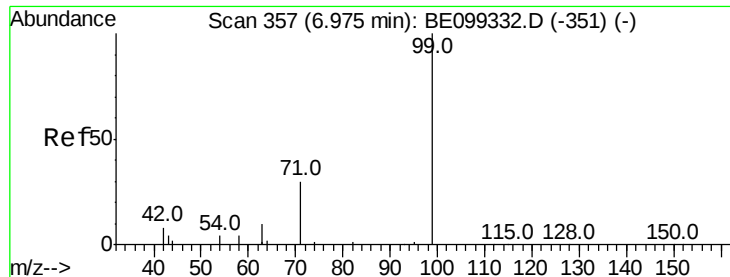

#5

Phenol-d6

Concen: 0.338 ng

RT: 6.98 min Scan# 357

Delta R.T. -0.00 min

Lab File: BE099385.D

Acq: 26 Apr 2019 19:19

Instrument :

BNA_E





ClientSampleId :

PST-003-SW024-042319

Tot Ion:	99	Resp:	4923
Ion	Ratio	Lower	Upper
99	100		
42	20.1	11.7	17.5#
71	42.7	29.6	44.4

Manual Integrations
APPROVED

Sohil
4/29/2019 1:28:50 PM



#7

Naphthalene-d8

Concen: 0.400 ng




RT: 10.61 min Scan# 650

Delta R.T. 0.01 min

Lab File: BE099385.D

Acq: 26 Apr 2019 19:19

Tgt Ion:	136	Resp:	16136
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.7	13.1
54	16.0	23.8	35.8#
68	4.0	6.4	9.6#





#8

Nitrobenzene-d5

Concen: 0.326 ng

RT: 8.98 min Scan# 524

Delta R.T. 0.01 min

Lab File: BE099385.D

Acq: 26 Apr 2019 19:19

Instrument :

BNA_E





ClientSampleId :

PST-003-SW024-042319

Tot Ion	Ratio	Lower	Upper
82	100		
128	159.7	91.7	137.5#
54	123.9	122.8	184.2

Manual Integrations
APPROVED

Sohil
4/29/2019 1:28:50 PM



#9

Naphthalene

Concen: 0.249 ng




RT: 10.65 min Scan# 653


Delta R.T. -0.00 min

Lab File: BE099385.D

Acq: 26 Apr 2019 19:19

Tgt Ion	Ratio	Lower	Upper
128	100		
129	3.0	2.3	3.5
127	3.5	2.8	4.2









#11
 2-Methylnaphthalene-d10
 Concen: 0.263 ng
 RT: 12.21 min Scan# 763
 Delta R.T. 0.01 min
 Lab File: BE099385.D
 Acq: 26 Apr 2019 19:19

Instrument :
 BNA_E
 ClientSampleId :
 PST-003-SW024-042319

Tot Ion	Ratio	Lower	Upper
152	100		
151	18.9	14.9	22.3




Manual Integrations
 APPROVED


Sohil
 4/29/2019 1:28:50 PM



#12
 2-Methylnaphthalene
 Concen: 0.209 ng
 RT: 12.28 min Scan# 768
 Delta R.T. 0.01 min
 Lab File: BE099385.D
 Acq: 26 Apr 2019 19:19

Tgt Ion	Ratio	Lower	Upper
142	100		
141	86.5	72.0	108.0
115	41.0	33.4	50.0





#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.46 min Scan# 919

Delta R.T. -0.00 min

Lab File: BE099385.D

Acq: 26 Apr 2019 19:19

Instrument :

BNA_E


ClientSampleId :

PST-003-SW024-042319




Tot Ion:	164	Resp:	10969
Ion Ratio	Lower	Upper	
164	100		
162	100.5	77.8	116.6
160	46.9	37.1	55.7

Manual Integrations
APPROVED

Sohil
4/29/2019 1:28:50 PM



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E



#14

2,4,6-Tribromophenol

Concen: 0.470 ng

RT: 15.94 min Scan# 1024




Delta R.T. -0.00 min


Lab File: BE099385.D

Acq: 26 Apr 2019 19:19

Tgt Ion:	330	Resp:	1712
Ion Ratio	Lower	Upper	
330	100		
332	93.9	82.5	123.7
141	28.7	24.9	37.3

Abundance Ion 330.00 (329.70 to 330.70): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E









#15
2-Fluorobiphenyl
Concen: 0.257 ng
RT: 13.09 min Scan# 824
Delta R.T. -0.00 min
Lab File: BE099385.D
Acq: 26 Apr 2019 19:19

Instrument :
BNA_E
ClientSampleId :
PST-003-SW024-042319

Tot Ion	Ratio	Lower	Upper
172	100		
171	34.0	26.2	39.2
170	23.6	18.1	27.1




Manual Integrations
APPROVED


Sohil
4/29/2019 1:28:50 PM



#16
Acenaphthylene
Concen: 0.031 ng
RT: 14.18 min Scan# 900
Delta R.T. -0.00 min
Lab File: BE099385.D
Acq: 26 Apr 2019 19:19

Tgt Ion	Ratio	Lower	Upper
152	100		
151	25.1	15.5	23.3#
153	21.9	10.2	15.4#





#17

Acenaphthene

Concen: 0.224 ng

RT: 14.53 min Scan# 924

Delta R.T. 0.01 min

Lab File: BE099385.D

Acq: 26 Apr 2019 19:19

Instrument :

BNA_E


ClientSampleId :

PST-003-SW024-042319




Tot Ion:	154	Resp:	6852
Ion	Ratio	Lower	Upper
154	100		
153	119.8	94.7	142.1
152	57.6	46.4	69.6

Manual Integrations
APPROVED

Sohil
4/29/2019 1:28:50 PM



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E



#18

Fluorene

Concen: 0.164 ng


RT: 15.50 min Scan# 991

Delta R.T. 0.01 min



Lab File: BE099385.D


Acq: 26 Apr 2019 19:19

Tgt Ion:	166	Resp:	7193
Ion	Ratio	Lower	Upper
166	100		
165	98.0	79.7	119.5
167	15.2	11.0	16.4



Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.19 min Scan# 1117

Delta R.T. -0.00 min

Lab File: BE099385.D

Acq: 26 Apr 2019 19:19

Instrument :

BNA_E


ClientSampleId :

PST-003-SW024-042319

Tot Ion:	188	Resp:	29241
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	9.5	6.2	9.4#

Manual Integrations
APPROVED




Sohil
4/29/2019 1:28:50 PM



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0



#23

Phenanthrene

Concen: 1.855 ng


RT: 17.24 min Scan# 1121

Delta R.T. 0.01 min

Lab File: BE099385.D

Acq: 26 Apr 2019 19:19



Tgt Ion:	178	Resp:	143672
Ion Ratio	Lower	Upper	
178	100		
176	19.5	15.3	22.9
179	15.3	12.4	18.6




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E









#24
 Anthracene
 Concen: 0.292 ng
 RT: 17.32 min Scan# 1127
 Delta R.T. -0.00 min
 Lab File: BE099385.D
 Acq: 26 Apr 2019 19:19

Instrument :
 BNA_E
 ClientSampled :
 PST-003-SW024-042319

Tot Ion:178	Resp:	20123
Ion Ratio	Lower	Upper
178	100	
176	18.1	15.1 22.7
179	23.8	11.9 17.9#




Manual Integrations
 APPROVED


Sohil
 4/29/2019 1:28:50 PM



#25
 Fluoranthene-d10
 Concen: 0.252 ng
 RT: 19.22 min Scan# 1385
 Delta R.T. 0.01 min
 Lab File: BE099385.D
 Acq: 26 Apr 2019 19:19

Tgt Ion:212	Resp:	88416
Ion Ratio	Lower	Upper
212	100	
106	1.9	1.8 2.6
104	1.0	1.0 1.4









#26
 Fluoranthene
 Concen: 1.807 ng
 RT: 19.25 min Scan# 1390
 Delta R.T. 0.01 min
 Lab File: BE099385.D
 Acq: 26 Apr 2019 19:19

Instrument :
 BNA_E
 ClientSampleId :
 PST-003-SW024-042319

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	6.7	6.4	9.6
203	17.6	13.5	20.3




Manual Integrations
 APPROVED


Sohil
 4/29/2019 1:28:50 PM



#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.37 min Scan# 1630
 Delta R.T. 0.00 min
 Lab File: BE099385.D
 Acq: 26 Apr 2019 19:19

Tgt Ion	Ratio	Resp Lower	Upper
240	100		
120	5.3	2.2	3.2#
236	28.1	20.2	30.4





#28

Pvrene

Concen: 1.690 ng

RT: 19.62 min Scan# 1453

Delta R.T. 0.01 min

Lab File: BE099385.D

Acq: 26 Apr 2019 19:19

Instrument :

BNA_E


ClientSampleId :

PST-003-SW024-042319




Tot Ion:	202	Resp:	160477
Ion Ratio	Lower	Upper	
202	100		
200	19.9	15.7	23.5
203	21.6	13.7	20.5

Manual Integrations
APPROVED

Sohil
4/29/2019 1:28:50 PM



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E



#29

Terphenyl-d14

Concen: 0.297 ng

RT: 19.82 min Scan# 1488




Delta R.T. 0.00 min


Lab File: BE099385.D

Acq: 26 Apr 2019 19:19

Tgt Ion:	244	Resp:	18857
Ion Ratio	Lower	Upper	
244	100		
212	32.3	22.6	33.8
122	7.0	4.6	7.0

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E






#30
Benzo(a)anthracene
Concen: 1.010 ng
RT: 21.36 min Scan# 1629
Delta R.T. 0.01 min
Lab File: BE099385.D
Acq: 26 Apr 2019 19:19

Instrument :
BNA_E
ClientSampleId :
PST-003-SW024-042319

Tot Ion	Ratio	Lower	Upper
228	100		
226	27.2	22.0	33.0
229	21.6	15.8	23.8

Manual Integrations
APPROVED

Sohil
4/29/2019 1:28:50 PM






Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



#31
Chrysene
Concen: 0.777 ng
RT: 21.40 min Scan# 1633
Delta R.T. 0.00 min
Lab File: BE099385.D
Acq: 26 Apr 2019 19:19




Tgt Ion	Ratio	Lower	Upper
228	100		
226	31.0	23.4	35.2
229	23.2	16.2	24.2


Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E





#32

Bis(2-ethylhexyl)phthalate

Concen: 0.191 ng

RT: 21.27 min Scan# 1622

Delta R.T. 0.00 min

Lab File: BE099385.D

Acq: 26 Apr 2019 19:19

Instrument :

BNA_E


ClientSampleId :

PST-003-SW024-042319




Tot Ion:	149	Resp:	16482
Ion Ratio	Lower	Upper	
149	100		
167	7.4	6.0	9.0
279	1.9	1.1	1.7#

Manual Integrations
APPROVED

Sohil
4/29/2019 1:28:50 PM



Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E



#33

Indeno(1,2,3-cd)pyrene

Concen: 0.362 ng

RT: 26.52 min Scan# 2938




Delta R.T. 0.02 min


Lab File: BE099385.D

Acq: 26 Apr 2019 19:19

Tgt Ion:	276	Resp:	36088
Ion Ratio	Lower	Upper	
276	100		
138	10.1	12.7	19.1#
277	22.2	19.6	29.4

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E









#34
Pervlene-d12
Concen: 0.400 ng
RT: 23.87 min Scan# 2201
Delta R.T. 0.01 min
Lab File: BE099385.D
Acq: 26 Apr 2019 19:19

Instrument :
BNA_E
ClientSampleId :
PST-003-SW024-042319

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.6	20.1	30.1
265	28.2	19.9	29.9




Manual Integrations
APPROVED


Sohil
4/29/2019 1:28:50 PM



#35
Benzo(b)fluoranthene
Concen: 0.831 ng
RT: 23.10 min Scan# 1985
Delta R.T. 0.02 min
Lab File: BE099385.D
Acq: 26 Apr 2019 19:19

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.2	17.3	25.9
125	8.3	5.8	8.6









#36
Benzo(k)fluoranthene
Concen: 0.275 ng m
RT: 23.15 min Scan# 1997
Delta R.T. 0.01 min
Lab File: BE099385.D
Acq: 26 Apr 2019 19:19

Instrument :
BNA_E
ClientSampleId :
PST-003-SW024-042319

Tot Ion	Ratio	Lower	Upper
252	100		
253	25.3	18.4	27.6
125	9.0	5.4	8.0




Manual Integrations
APPROVED


Sohil
4/29/2019 1:28:50 PM



#37
Benzo(a)pyrene
Concen: 0.663 ng
RT: 23.75 min Scan# 2168
Delta R.T. 0.01 min
Lab File: BE099385.D
Acq: 26 Apr 2019 19:19

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.5	17.6	26.4
125	8.1	6.5	9.7









#38
Dibenzo(a,h)anthracene
Concen: 0.085 ng
RT: 26.54 min Scan# 2945
Delta R.T. 0.02 min
Lab File: BE099385.D
Acq: 26 Apr 2019 19:19

Instrument :
BNA_E
ClientSampleId :
PST-003-SW024-042319

Tot Ion	Ratio	Lower	Upper
278	100		
139	21.0	8.5	12.7#
279	36.9	19.8	29.8#

Manual Integrations
APPROVED

Sohil
4/29/2019 1:28:50 PM



#39
Benzo(g,h,i)perylene
Concen: 0.313 ng
RT: 27.34 min Scan# 3168
Delta R.T. 0.03 min
Lab File: BE099385.D
Acq: 26 Apr 2019 19:19

Tgt Ion	Ratio	Lower	Upper
276	100		
277	27.1	20.0	30.0
138	13.6	11.1	16.7

