


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE042619\
 Data File : BE099369.D
 Acq On : 26 Apr 2019 9:42
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 19 06:51:38 2019

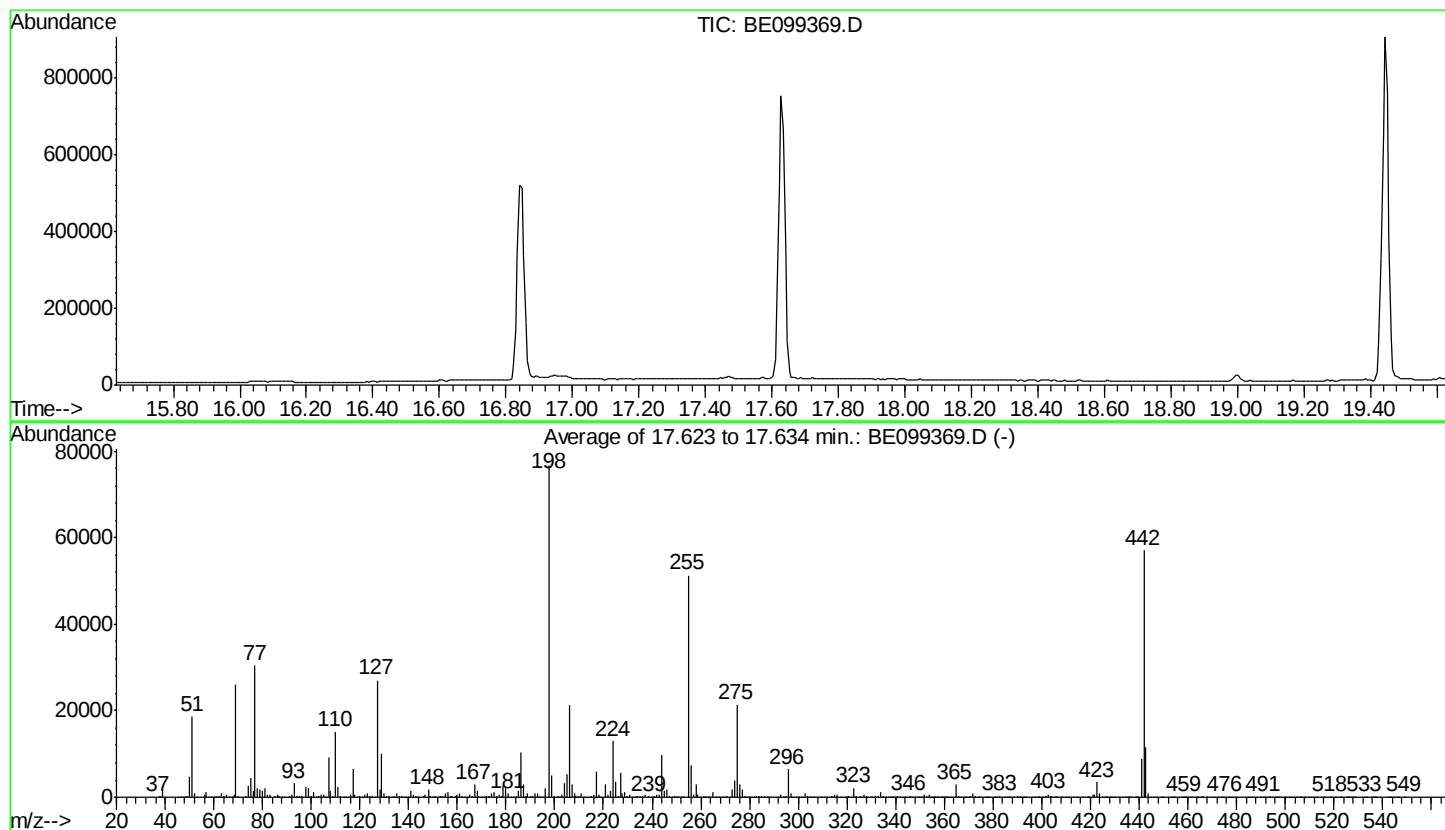

AutoFind: Scans 2559, 2560, 2561; Background Corrected with Scan 2552

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.1	18513	PASS
68	69	0.00	2	1.8	461	PASS
69	198	0.00	100	33.9	25975	PASS
70	69	0.00	2	0.7	182	PASS
127	198	10	80	35.3	27050	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76685	PASS
199	198	5	9	6.6	5098	PASS
275	198	10	60	27.8	21334	PASS
365	198	1	100	3.8	2933	PASS
441	198	0.01	100	11.6	8912	PASS
442	198	50	100	74.4	57029	PASS
443	442	15	24	20.3	11573	PASS