


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE042619\
Data File : BE099387.D
Acq On : 26 Apr 2019 21:07
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041819.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 19 06:51:38 2019

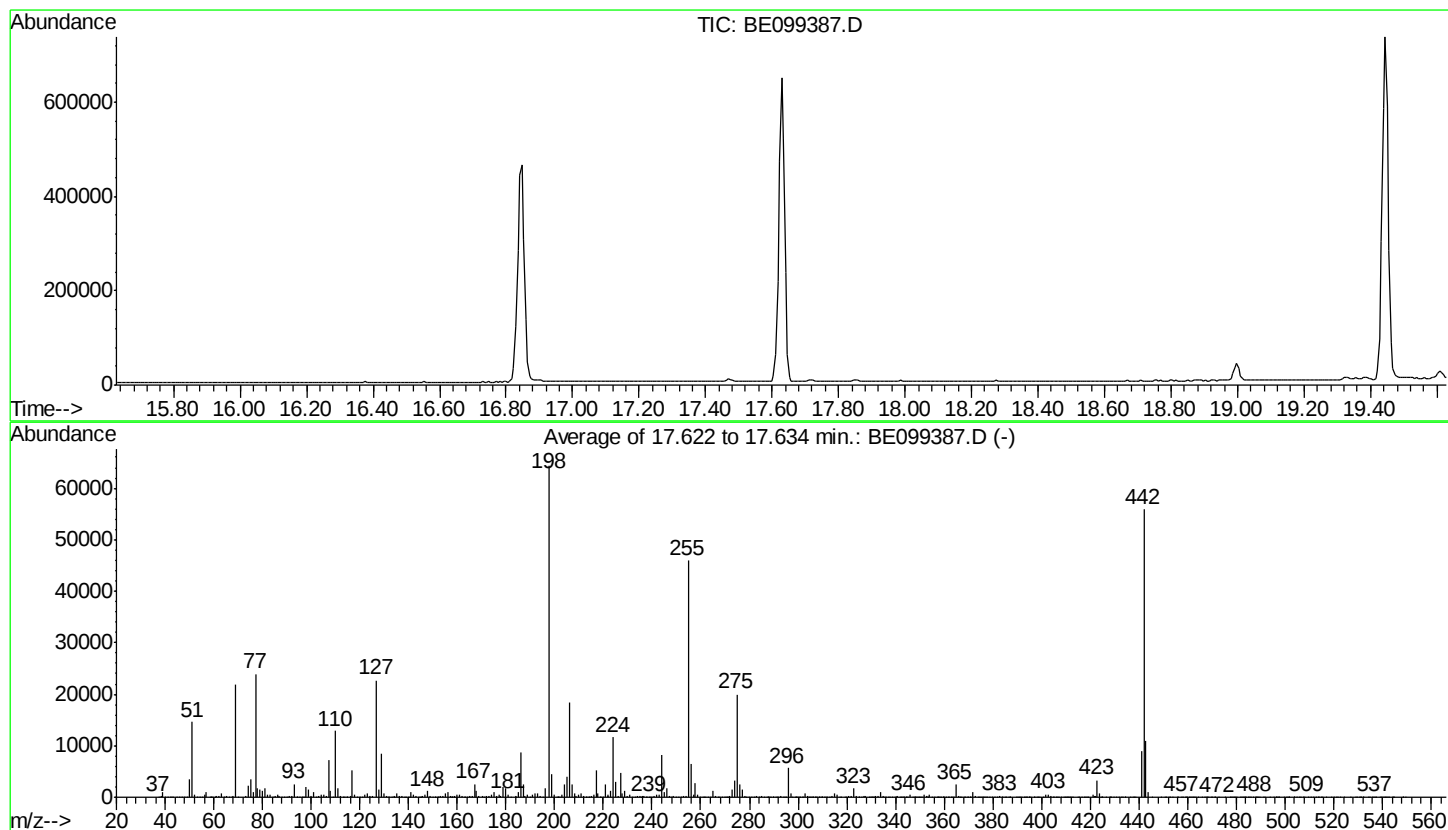

AutoFind: Scans 2559, 2560, 2561; Background Corrected with Scan 2551

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.7	14629	PASS
68	69	0.00	2	0.8	177	PASS
69	198	0.00	100	34.0	21876	PASS
70	69	0.00	2	0.6	128	PASS
127	198	10	80	35.3	22732	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64383	PASS
199	198	5	9	7.1	4551	PASS
275	198	10	60	31.0	19962	PASS
365	198	1	100	3.8	2468	PASS
441	198	0.01	100	14.0	9008	PASS
442	198	50	100	86.7	55819	PASS
443	442	15	24	19.6	10962	PASS