


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE050119\
 Data File : BE099453.D
 Acq On : 1 May 2019 8:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE042919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 29 18:36:43 2019

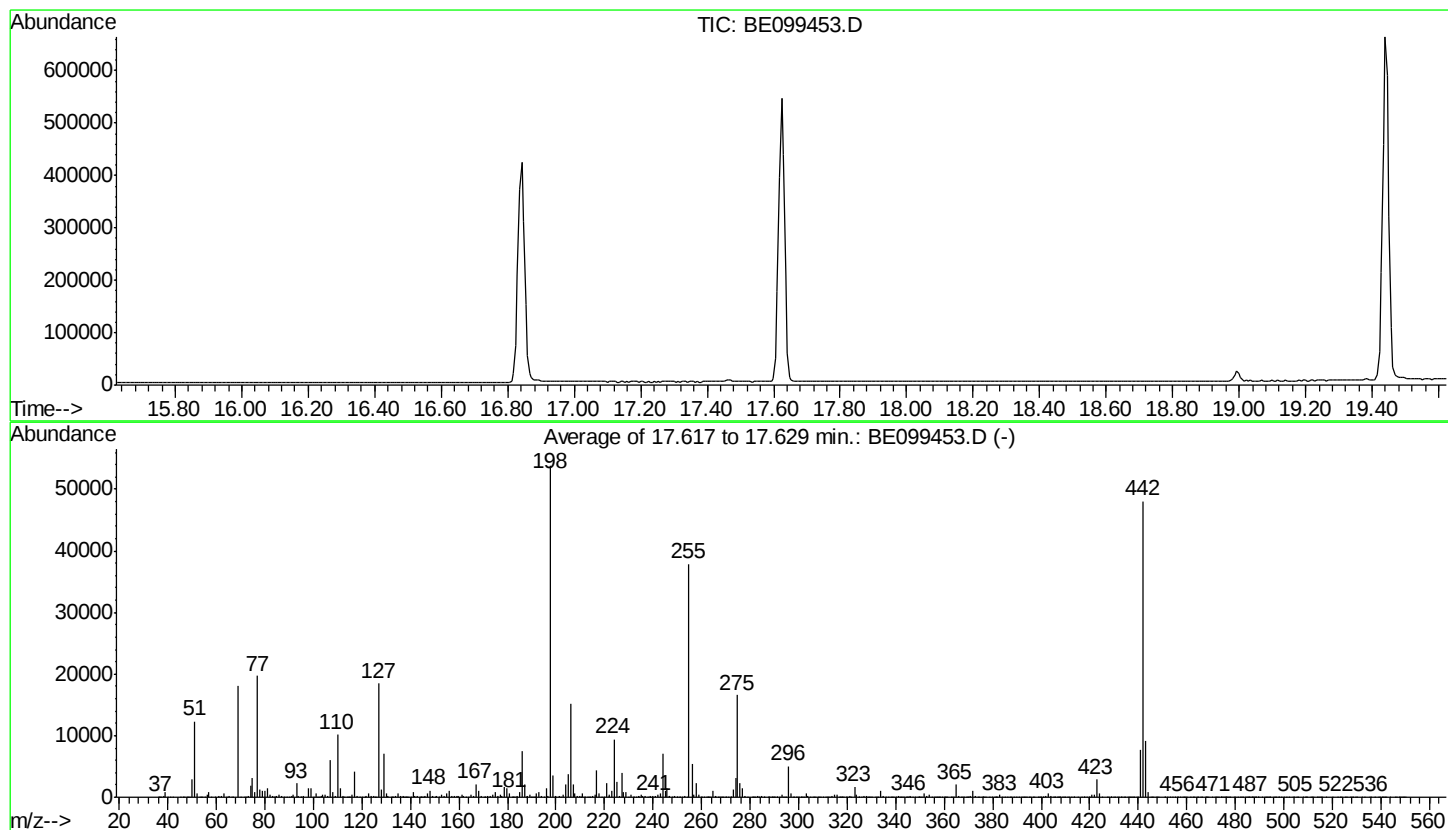

AutoFind: Scans 2558, 2559, 2560; Background Corrected with Scan 2551

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.9	12336	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.6	18065	PASS
70	69	0.00	2	0.5	97	PASS
127	198	10	80	34.2	18400	PASS
197	198	0.00	2	0.2	132	PASS
198	198	100	100	100.0	53826	PASS
199	198	5	9	6.5	3477	PASS
275	198	10	60	30.8	16594	PASS
365	198	1	100	3.7	2006	PASS
441	198	0.01	100	14.2	7670	PASS
442	198	50	100	89.4	48098	PASS
443	442	15	24	19.0	9142	PASS