


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE050119\
 Data File : BE099472.D
 Acq On : 1 May 2019 20:44
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE042919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 29 18:36:43 2019

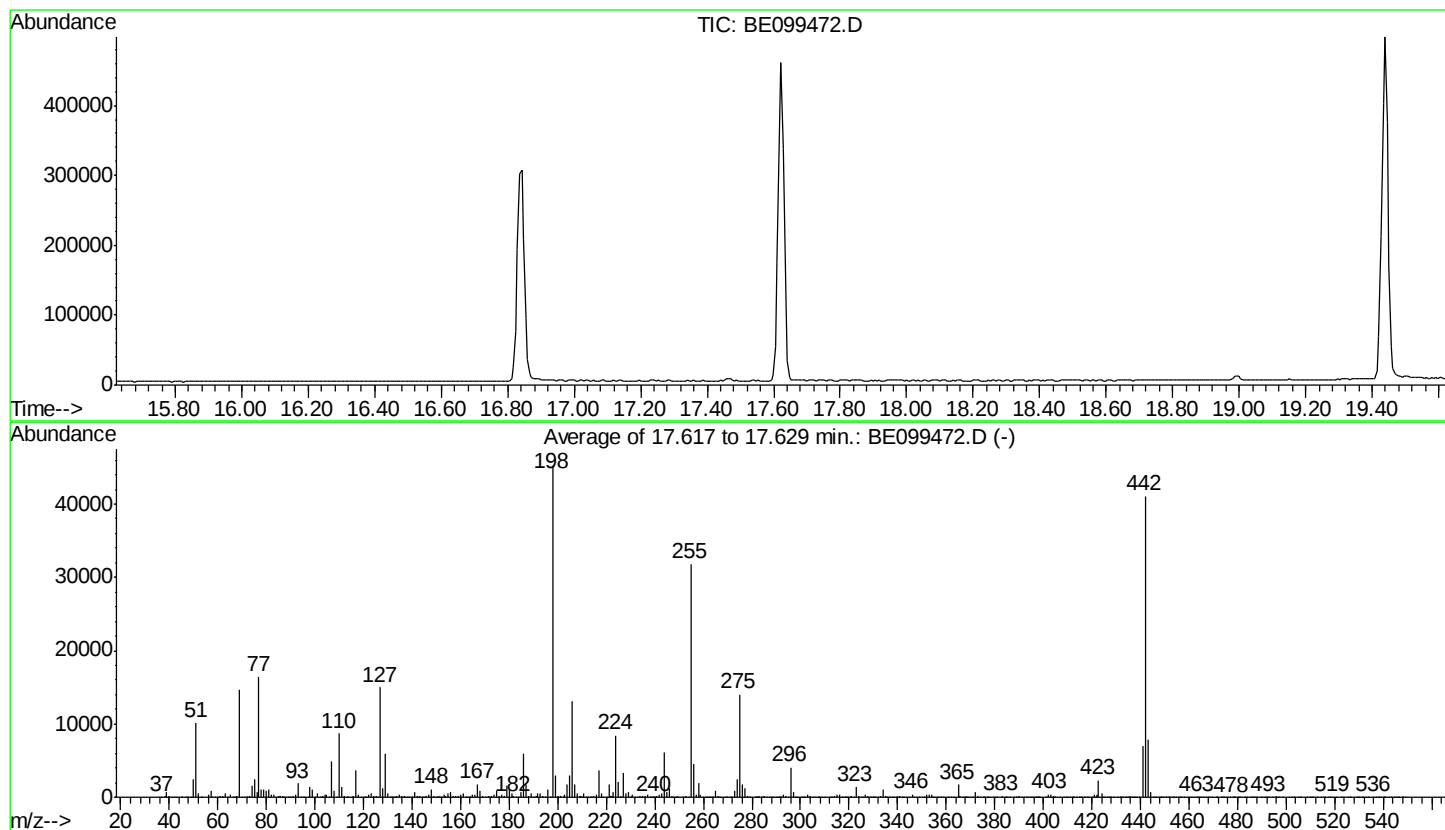

AutoFind: Scans 2558, 2559, 2560; Background Corrected with Scan 2551

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.4	10140	PASS
68	69	0.00	2	1.5	223	PASS
69	198	0.00	100	32.6	14733	PASS
70	69	0.00	2	0.3	38	PASS
127	198	10	80	33.1	14979	PASS
197	198	0.00	2	0.1	66	PASS
198	198	100	100	100.0	45245	PASS
199	198	5	9	6.5	2942	PASS
275	198	10	60	31.1	14050	PASS
365	198	1	100	3.8	1717	PASS
441	198	0.01	100	15.3	6926	PASS
442	198	50	100	90.7	41048	PASS
443	442	15	24	19.3	7940	PASS