


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE050719\
 Data File : BE099556.D
 Acq On : 7 May 2019 8:24
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE050719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 07 14:10:11 2019

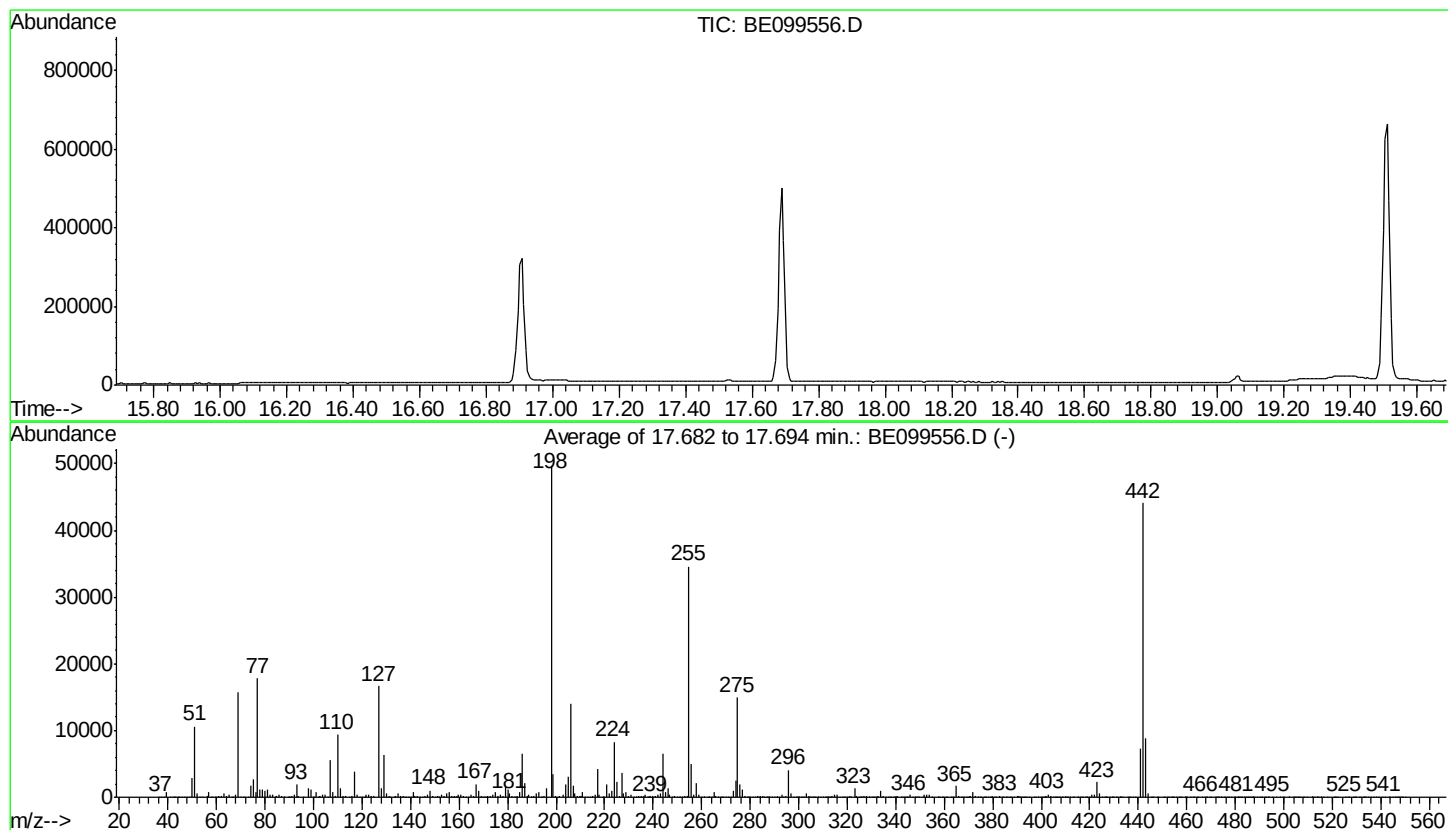

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2560

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.4	10640	PASS
68	69	0.00	2	2.0	318	PASS
69	198	0.00	100	31.7	15736	PASS
70	69	0.00	2	0.3	47	PASS
127	198	10	80	33.4	16616	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49706	PASS
199	198	5	9	6.9	3435	PASS
275	198	10	60	30.0	14921	PASS
365	198	1	100	3.4	1713	PASS
441	198	0.01	100	14.8	7335	PASS
442	198	50	100	88.6	44050	PASS
443	442	15	24	20.1	8852	PASS