


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE050819\
 Data File : BE099572.D
 Acq On : 8 May 2019 8:10
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE050719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 07 14:10:11 2019

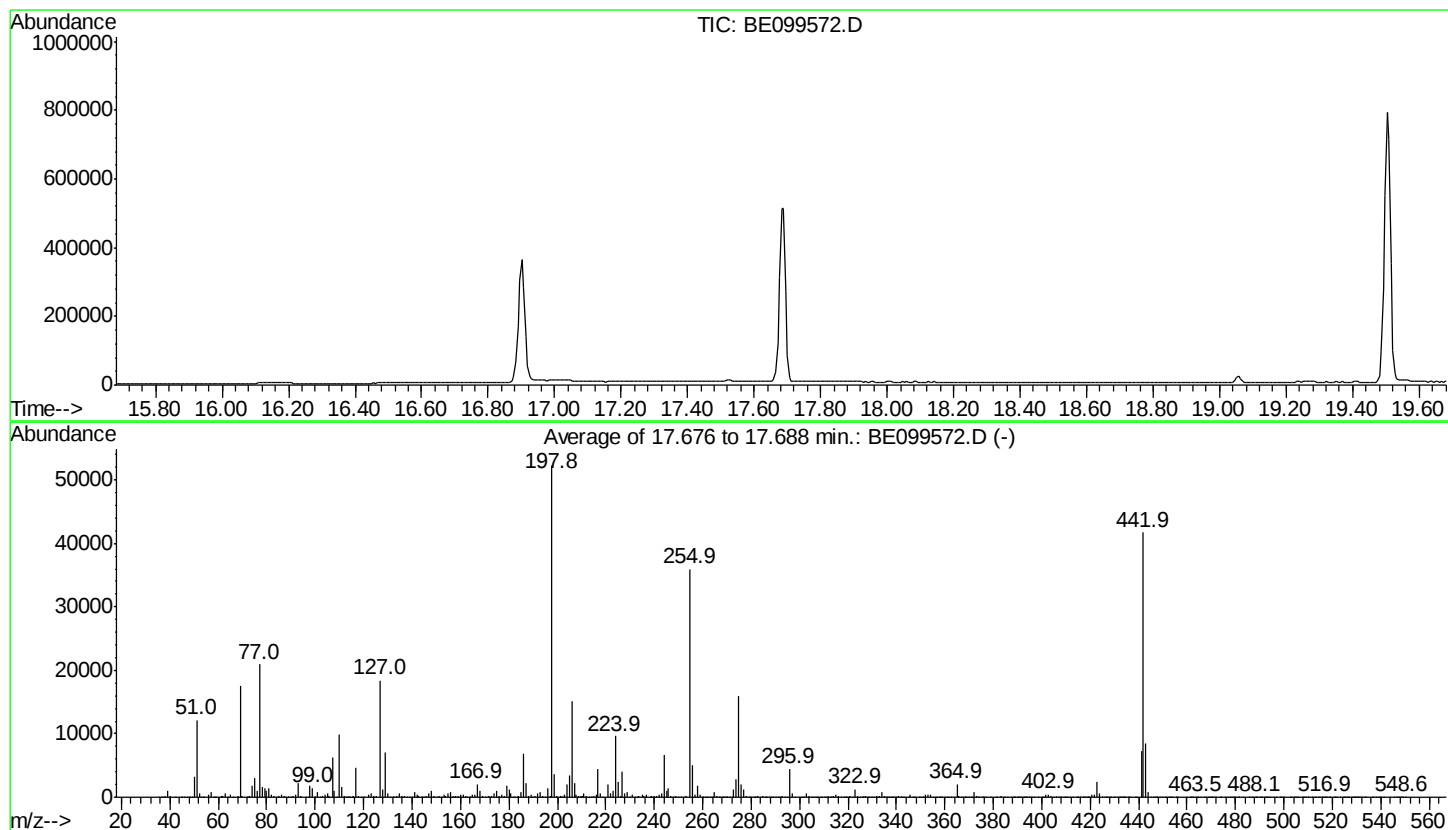

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2560

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.2	12148	PASS
68	69	0.00	2	0.8	134	PASS
69	198	0.00	100	33.5	17525	PASS
70	69	0.00	2	0.6	109	PASS
127	198	10	80	35.3	18462	PASS
197	198	0.00	2	0.3	133	PASS
198	198	100	100	100.0	52258	PASS
199	198	5	9	6.8	3552	PASS
275	198	10	60	30.4	15899	PASS
365	198	1	100	3.9	2021	PASS
441	198	0.01	100	13.7	7173	PASS
442	198	50	100	79.9	41732	PASS
443	442	15	24	20.3	8469	PASS