


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE050919\
 Data File : BE099580.D
 Acq On : 9 May 2019 8:08
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE050919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 09 13:32:58 2019

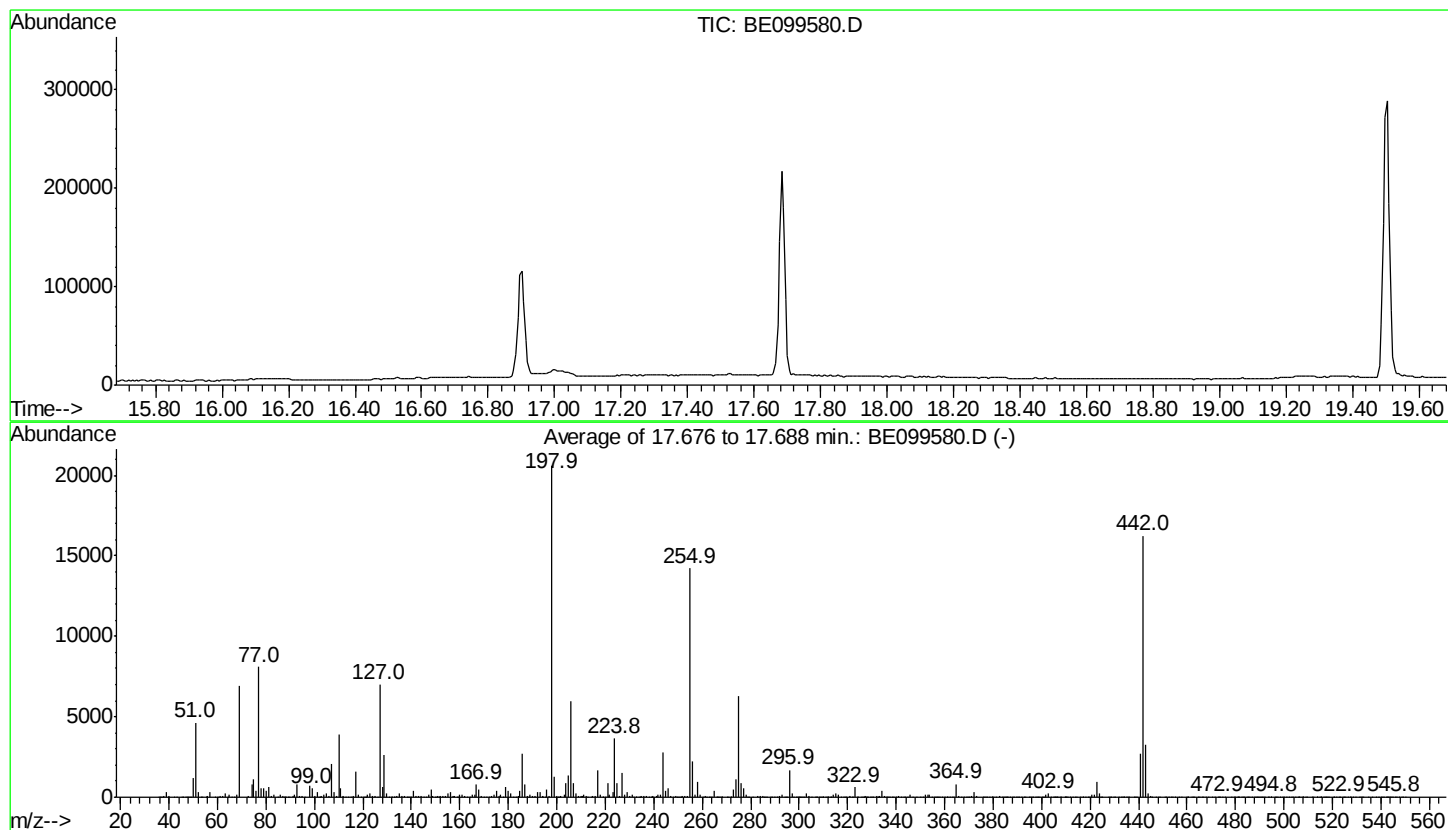

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.6	4653	PASS
68	69	0.00	2	1.8	127	PASS
69	198	0.00	100	33.4	6886	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.9	6976	PASS
197	198	0.00	2	0.4	90	PASS
198	198	100	100	100.0	20601	PASS
199	198	5	9	6.3	1289	PASS
275	198	10	60	30.7	6322	PASS
365	198	1	100	3.9	803	PASS
441	198	0.01	100	13.1	2706	PASS
442	198	50	100	78.9	16252	PASS
443	442	15	24	20.0	3250	PASS