
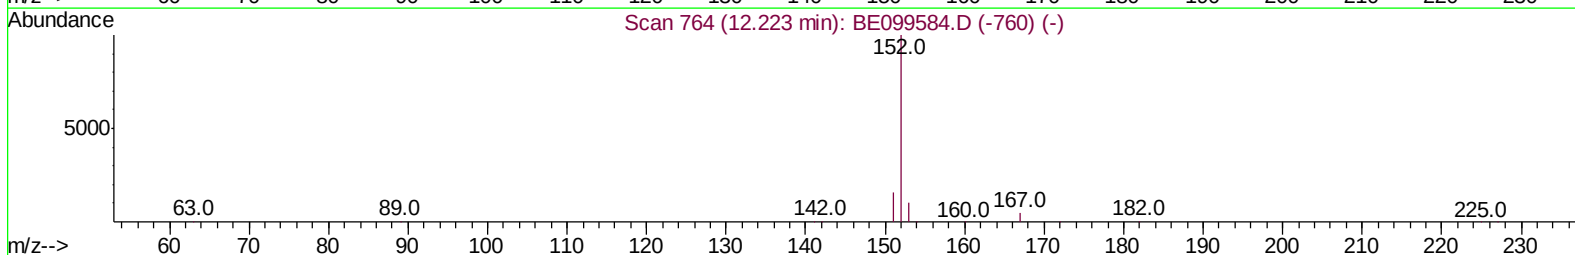
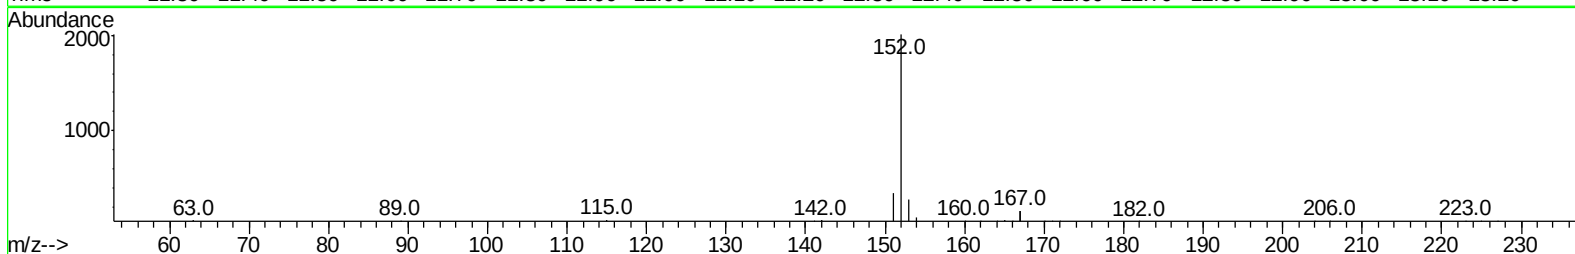


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE051019\
Data File : BE099598.D
Acq On : 10 May 2019 14:41
Operator : JU/SJ
Sample : PB119621BS
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB119621BS

Quant Time: May 11 01:00:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE050919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 09 13:32:58 2019
Response via : Initial Calibration

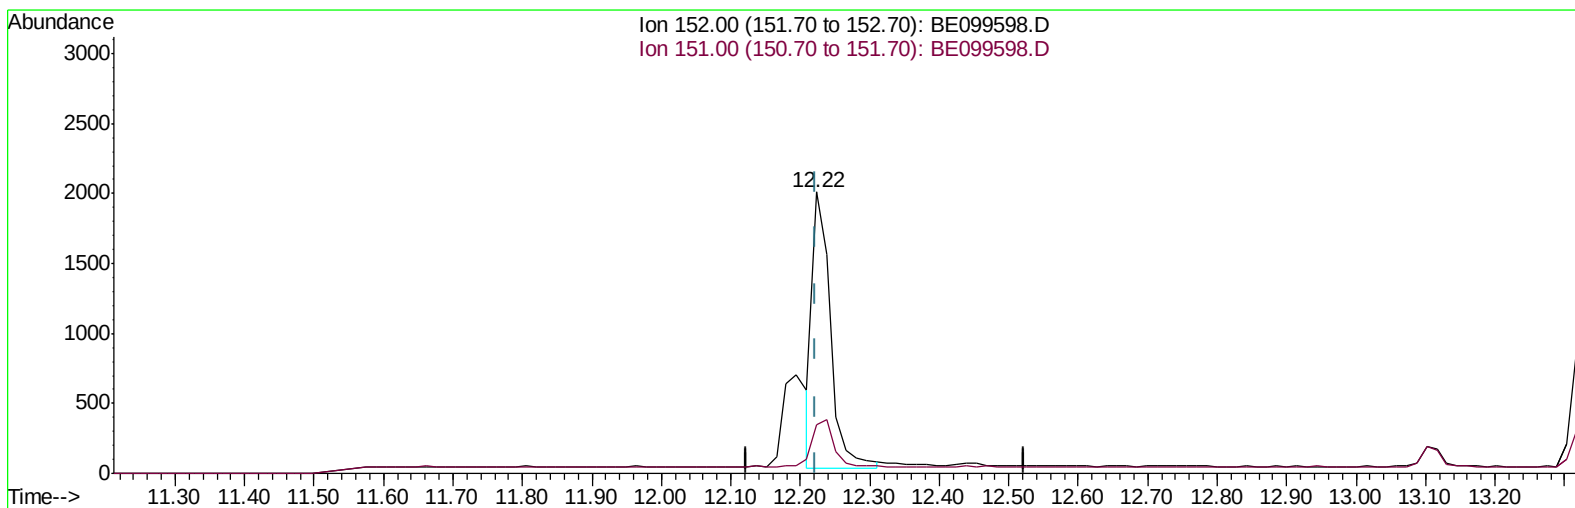

TIC: BE099598.D

(11) 2-Methylnaphthalene-d10 (SURR)

12.223min (+0.000) 0.31ng m

response 3579

Ion	Exp%	Act%
152.00	100	100
151.00	20.20	20.68
0.00	0.00	0.00
0.00	0.00	0.00