


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE051419\
 Data File : BE099604.D
 Acq On : 14 May 2019 14:41
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 14 19:30:50 2019

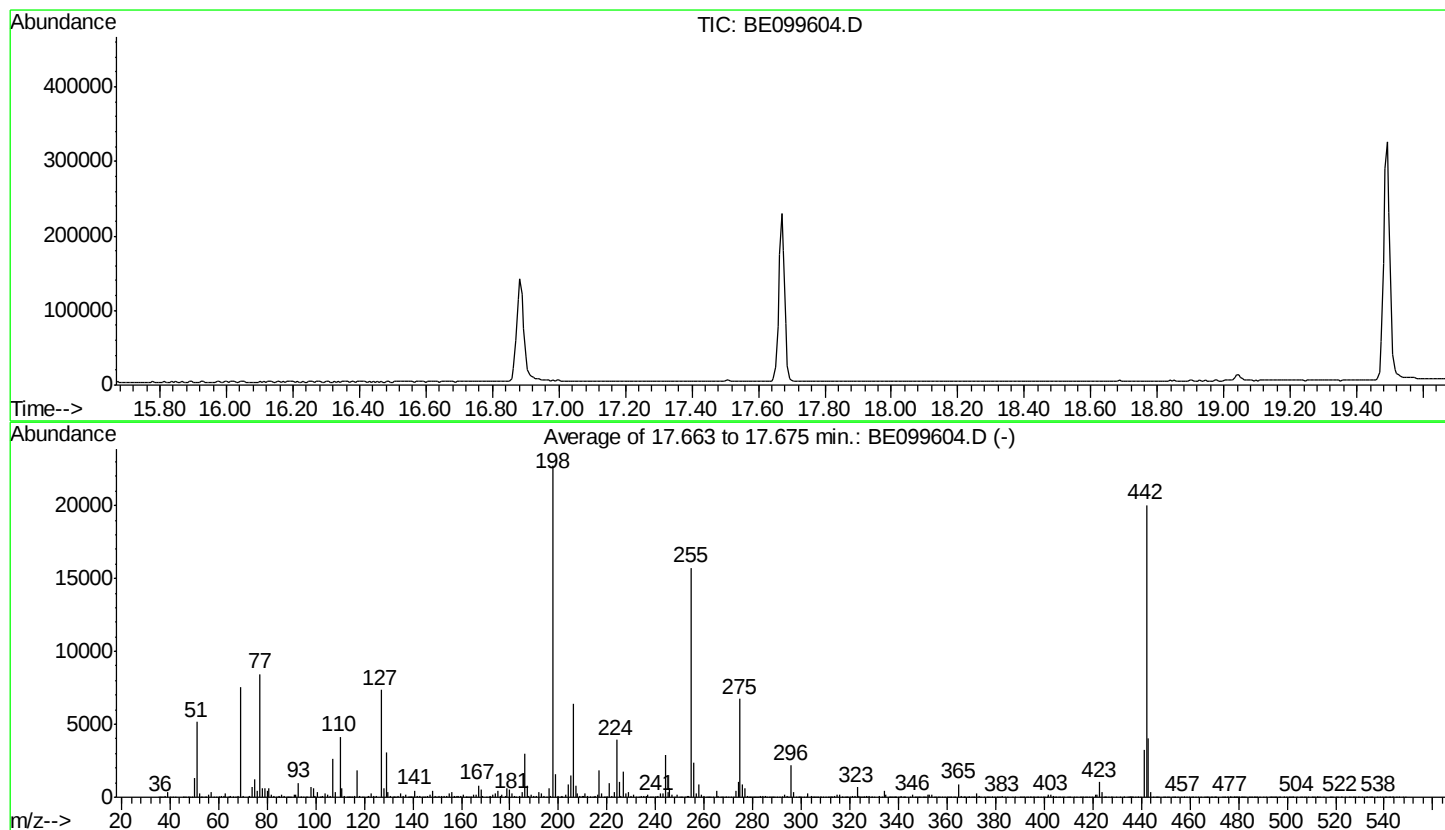

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.7	5164	PASS
68	69	0.00	2	1.0	76	PASS
69	198	0.00	100	33.3	7574	PASS
70	69	0.00	2	0.6	48	PASS
127	198	10	80	32.3	7354	PASS
197	198	0.00	2	0.4	91	PASS
198	198	100	100	100.0	22733	PASS
199	198	5	9	6.9	1563	PASS
275	198	10	60	29.6	6725	PASS
365	198	1	100	3.9	884	PASS
441	198	0.01	100	14.4	3282	PASS
442	198	50	100	88.1	20032	PASS
443	442	15	24	20.0	3999	PASS