


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE051518\
 Data File : BE096570.D
 Acq On : 15 May 2018 8:34
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 15 13:02:03 2018

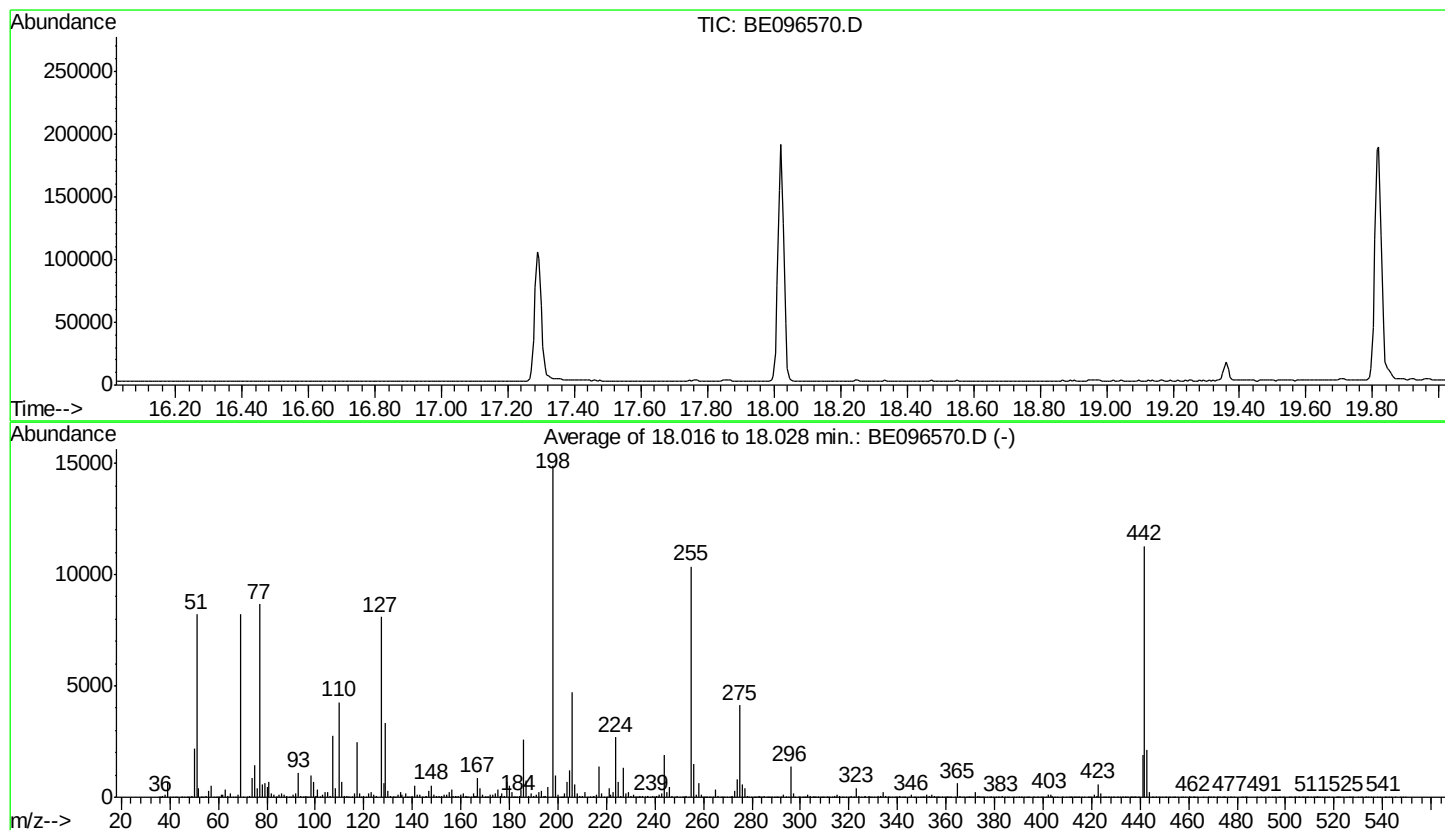

AutoFind: Scans 2626, 2627, 2628; Background Corrected with Scan 2618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.2	8216	PASS
68	69	0.00	2	1.4	113	PASS
69	198	0.00	100	55.1	8210	PASS
70	69	0.00	2	0.3	28	PASS
127	198	10	80	54.3	8082	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14894	PASS
199	198	5	9	6.5	972	PASS
275	198	10	60	27.6	4117	PASS
365	198	1	100	4.1	606	PASS
441	198	0.01	100	12.9	1920	PASS
442	198	50	100	75.8	11283	PASS
443	442	15	24	19.1	2154	PASS