
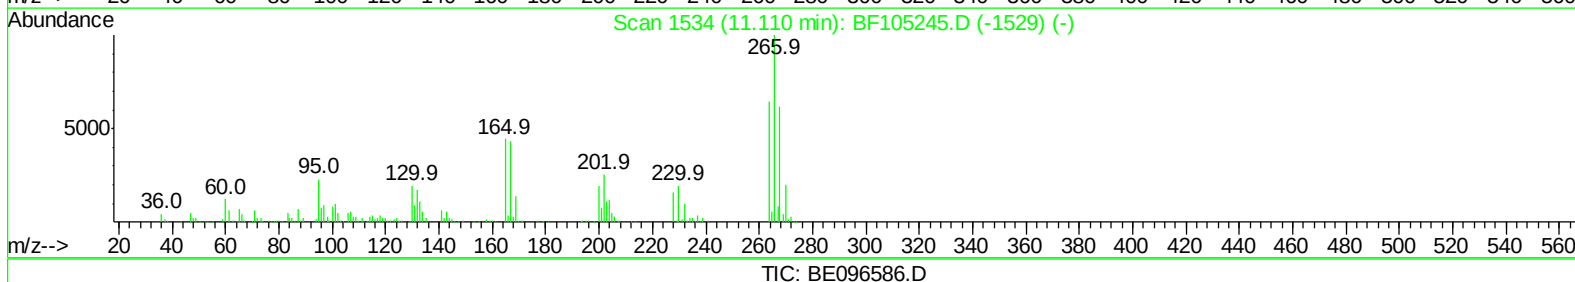
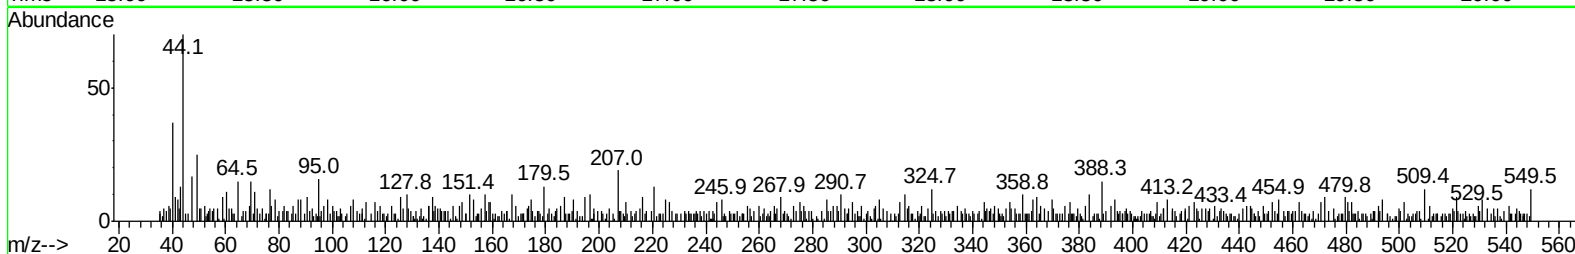


Data Path : Z:\HPCHEM1\BNA E\DATA\BE051618\
Data File : BE096586.D
Acq On : 16 May 2018 8:02
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 04:35:40 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 16 17:08:52 2018
Response via : Initial Calibration

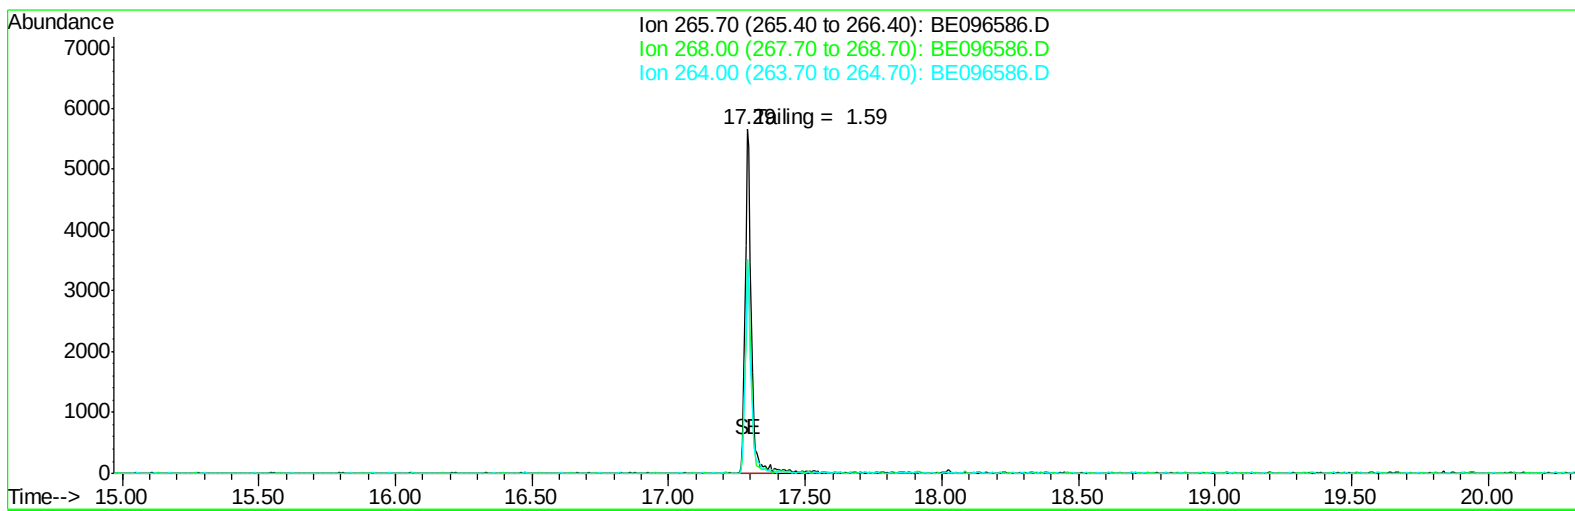

(69) Pentachlorophenol (C)




11.184min (+0.068) 80.22ng

response 8

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	75.00
264.00	61.90	50.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE051618\
Data File : BE096586.D
Acq On : 16 May 2018 8:02
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 04:35:40 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF051018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 16 17:08:52 2018
Response via : Initial Calibration

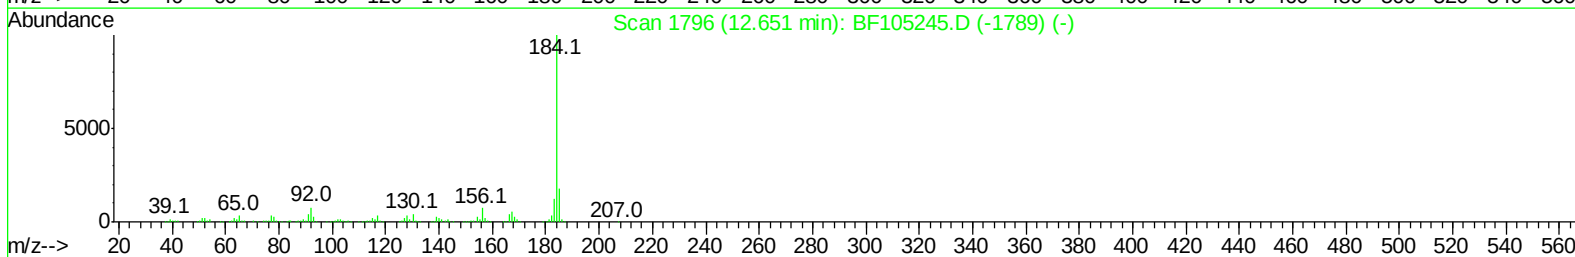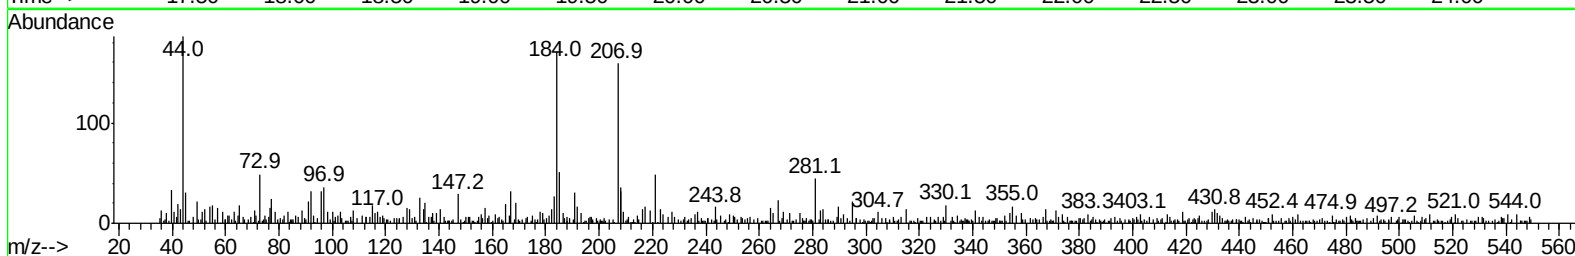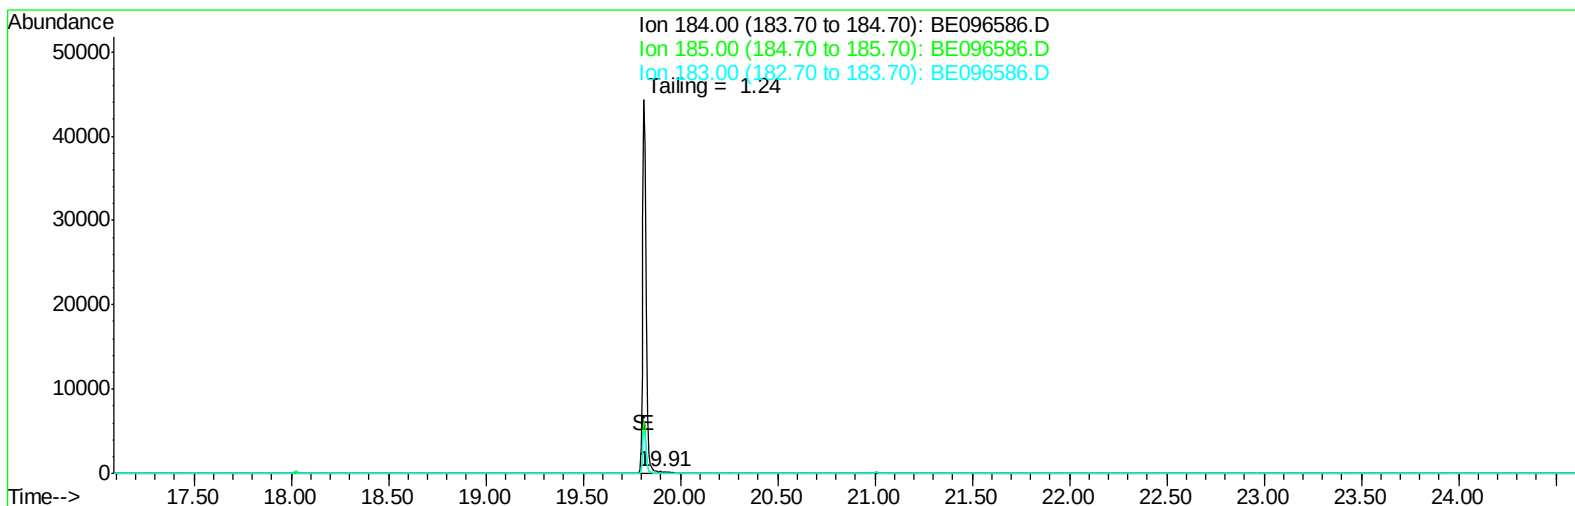

TIC: BE096586.D

(76) Benzidine

19.909min (+7.258) 714.76ng m

response 230

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	29.82#
183.00	11.60	15.79#
0.00	0.00	0.00