

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE051618\
 Data File : BE096588.D
 Acq On : 16 May 2018 9:16
 Operator : SJ/JU
 Sample : PB108420BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB108420BL

Quant Time: May 17 03:58:20 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 15 13:02:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.35	152	807	0.40	ng	0.00
7) Naphthalene-d8	11.18	136	3013	0.40	ng	0.00
13) Acenaphthene-d10	14.92	164	1537	0.40	ng	0.00
19) Phenanthrene-d10	17.64	188	3468	0.40	ng	0.00
27) Chrysene-d12	21.74	240	3687	0.40	ng	0.01
34) Perylene-d12	24.33	264	3524	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.86	112	892	0.40	ng	0.00
5) Phenol-d6	7.51	99	1105	0.35	ng	0.00
8) Nitrobenzene-d5	9.53	82	1150	0.36	ng	0.00
11) 2-Methylnaphthalene-d10	12.72	152	1624	0.33	ng	0.00
14) 2,4,6-Tribromophenol	16.40	330	189	0.31	ng	0.00
15) 2-Fluorobiphenyl	13.56	172	2403	0.36	ng	0.00
25) Fluoranthene-d10	19.62	212	15747	0.37	ng	0.00
29) Terphenyl-d14	20.18	244	2914	0.35	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE051618\
Data File : BE096588.D
Acq On : 16 May 2018 9:16
Operator : SJ/JU
Sample : PB108420BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB108420BL

Quant Time: May 17 03:58:20 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 15 13:02:03 2018
Response via : Initial Calibration

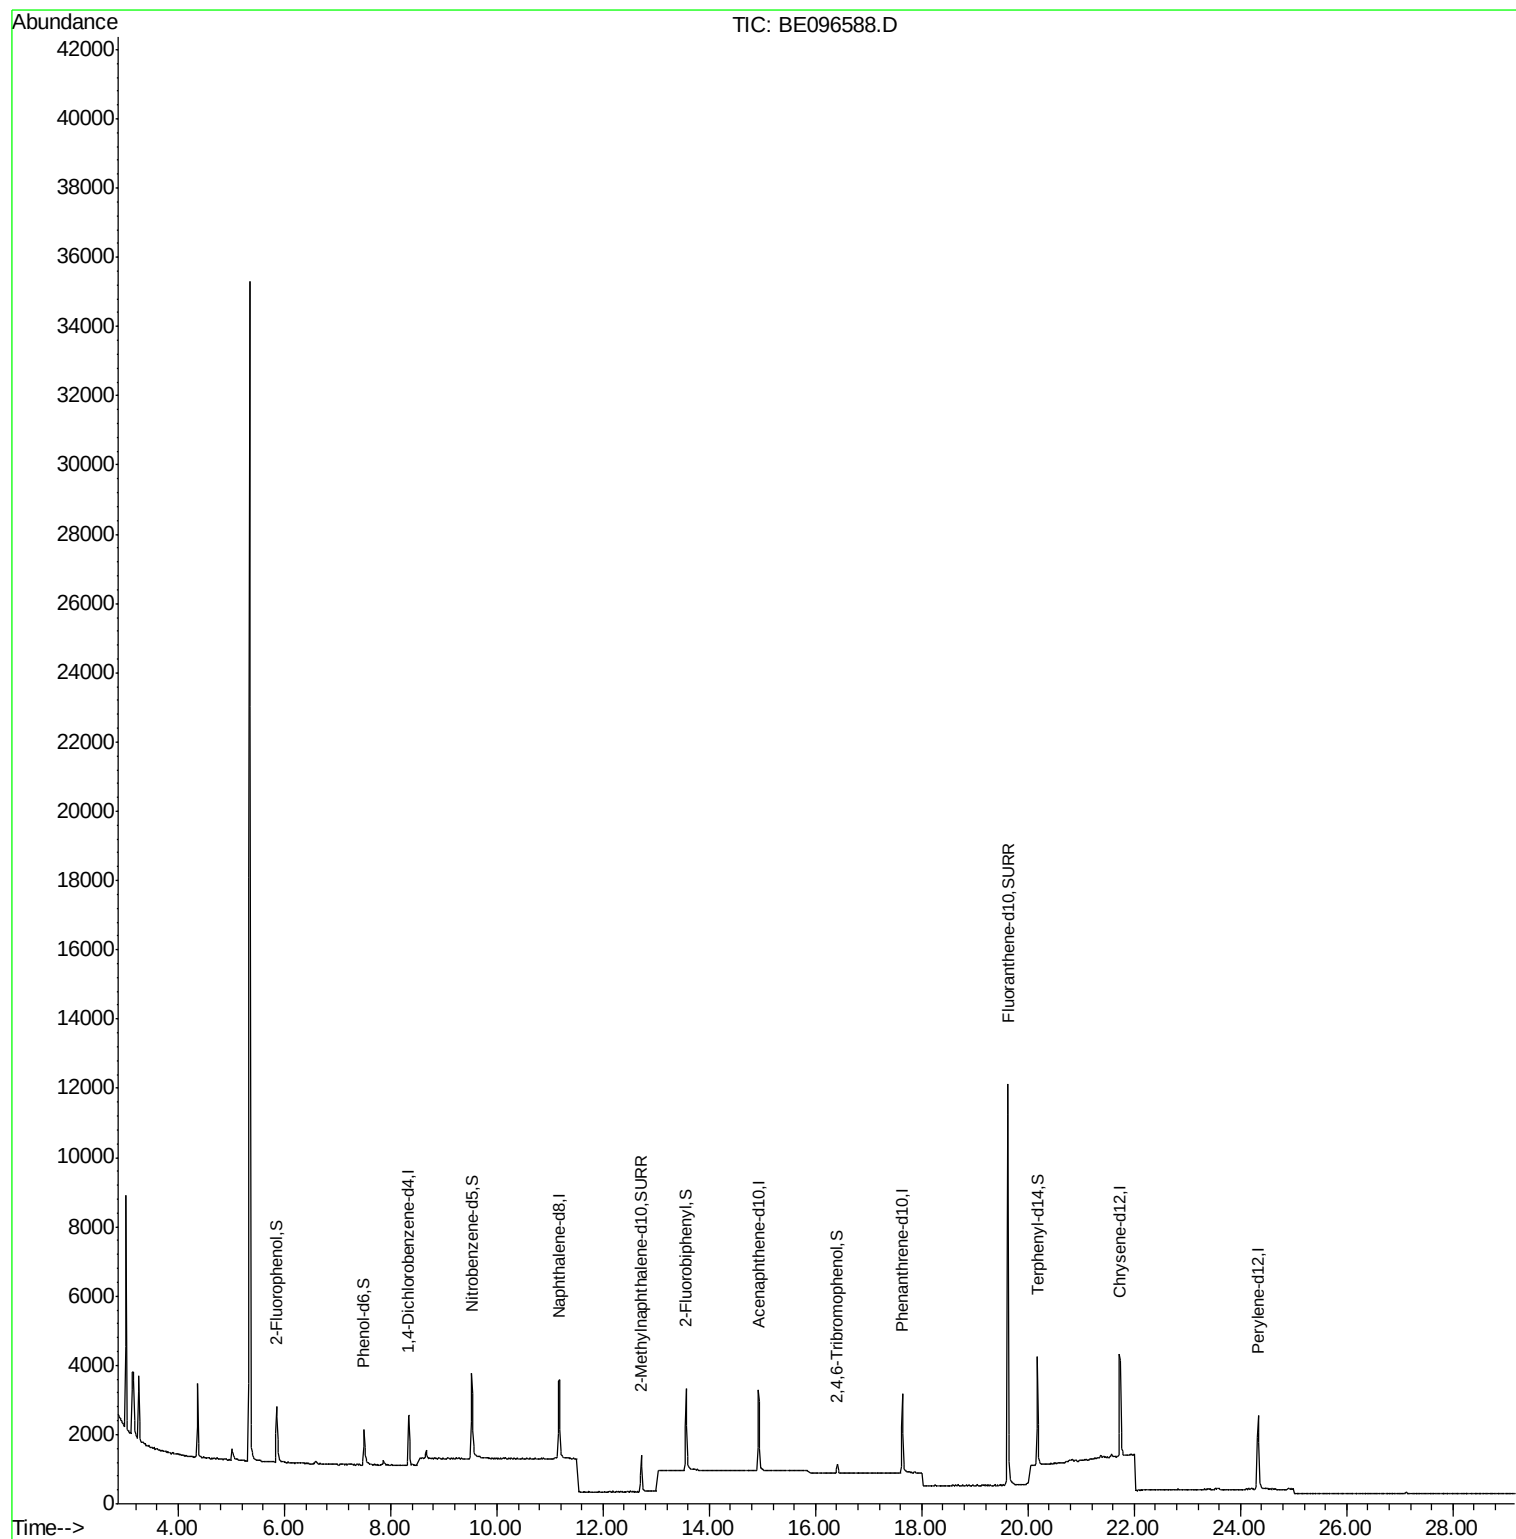

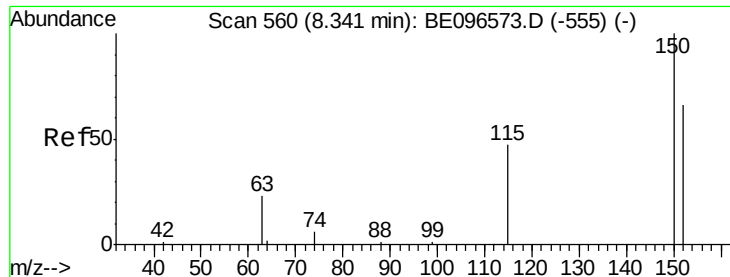


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.35 min Scan# 561
Delta R.T. 0.01 min
Lab File: BE096588.D
Acq: 16 May 2018 9:16

Instrument :
BNA_E
ClientSampleId :
PB108420BL

Tgt Ion:152 Resp: 807
Ion Ratio Lower Upper
152 100
150 137.4 117.2 175.8
115 67.3 57.0 85.6

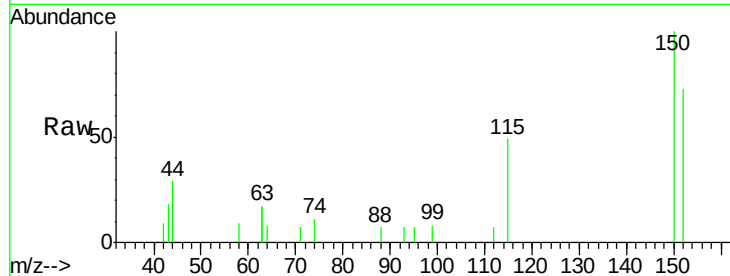


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

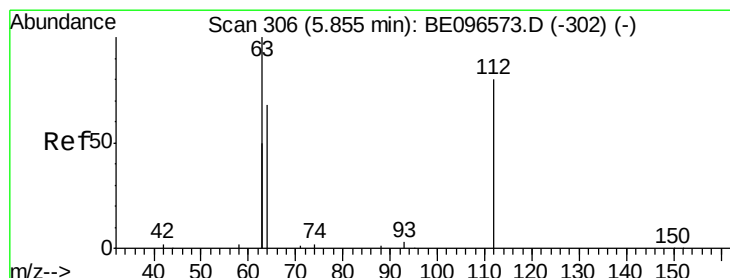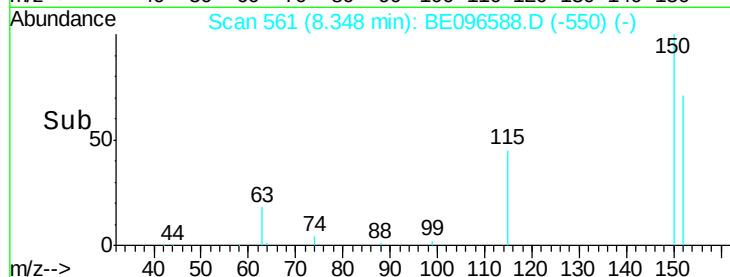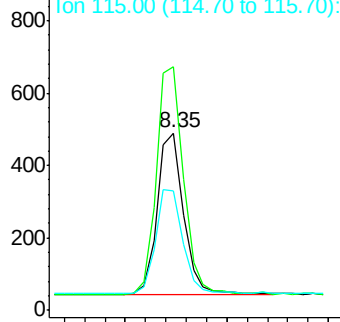



#4


2-Fluorophenol
Concen: 0.401 ng
RT: 5.86 min Scan# 307
Delta R.T. 0.01 min
Lab File: BE096588.D
Acq: 16 May 2018 9:16

Tgt Ion:112 Resp: 892
Ion Ratio Lower Upper
112 100
64 75.4 60.1 90.1
63 171.5 116.8 175.2

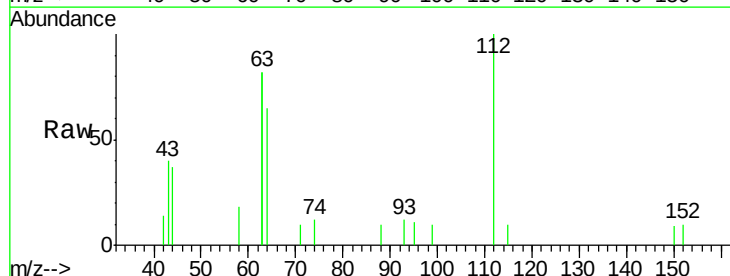

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BE0
Ion 63.00 (62.70 to 63.70): BE0

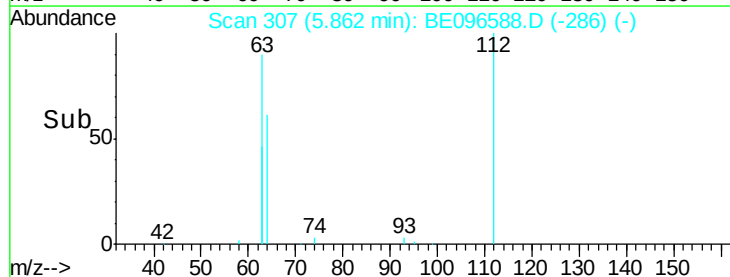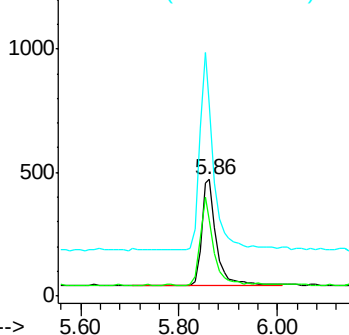

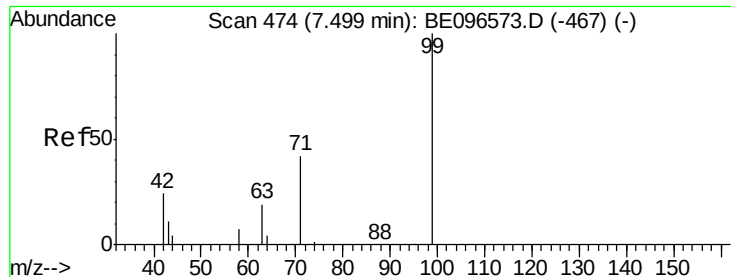

#5

Phenol-d6

Concen: 0.351 ng

RT: 7.51 min Scan# 475

Delta R.T. 0.01 min

Lab File: BE096588.D

Acq: 16 May 2018 9:16

Instrument :

BNA_E

ClientSampleId :

PB108420BL


Tgt Ion: 99 Resp: 1105

Ion Ratio Lower Upper

99 100

42 28.7 20.2 30.2




71 44.5 28.4 42.6#

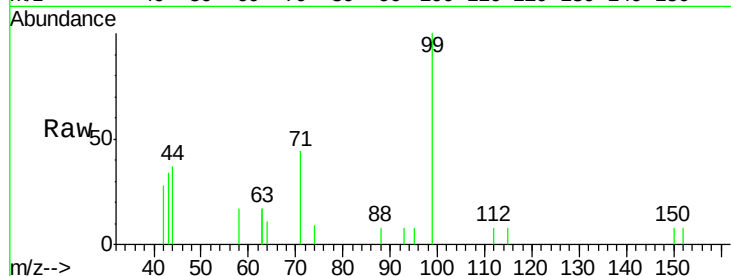

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

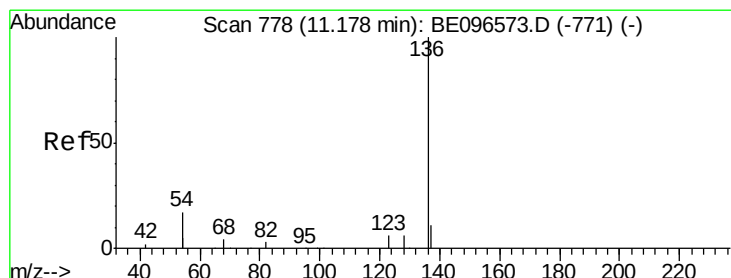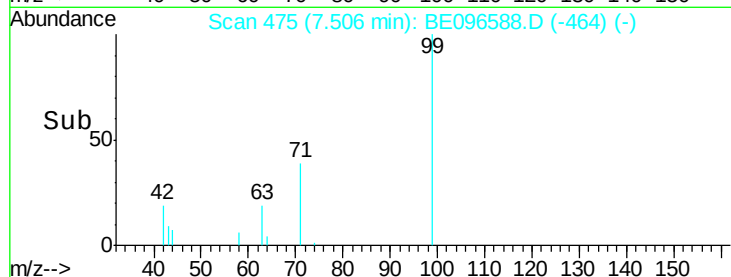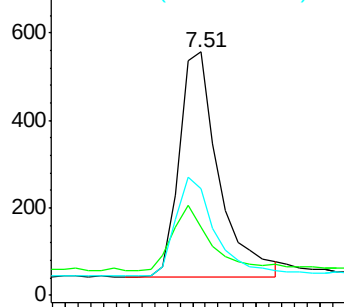

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 11.18 min Scan# 778

Delta R.T. -0.00 min

Lab File: BE096588.D

Acq: 16 May 2018 9:16

Tgt Ion: 136 Resp: 3013


Ion Ratio Lower Upper

136 100

137 13.9 9.5 14.3

54 37.7 29.1 43.7

68 7.3 6.2 9.2


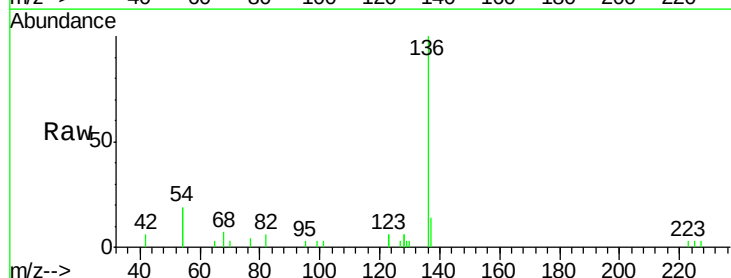



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

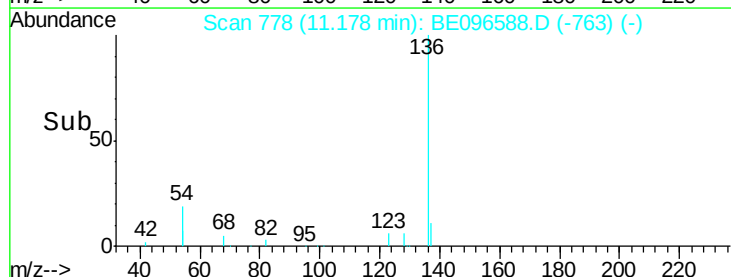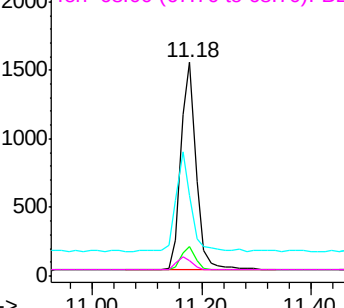

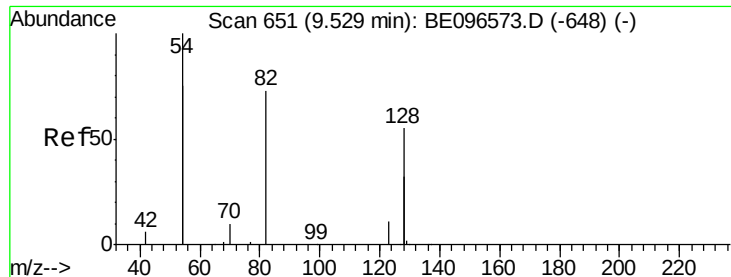

#8

Nitrobenzene-d5

Concen: 0.359 ng

RT: 9.53 min Scan# 651

Delta R.T. -0.00 min

Lab File: BE096588.D

Acq: 16 May 2018 9:16

Instrument :

BNA_E

ClientSampleId :

PB108420BL


Tgt Ion: 82 Resp: 1150

Ion Ratio Lower Upper

82 100

128 128.1 150.0 225.0#




54 254.9 154.2 231.4#

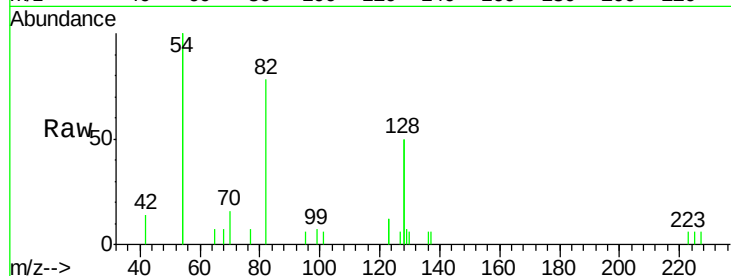

Abundance Ion 82.00 (81.70 to 82.70): BE096573.D (-648) (-)

Ion 128.00 (127.70 to 128.70): BE096573.D (-648) (-)

Ion 54.00 (53.70 to 54.70): BE096573.D (-648) (-)

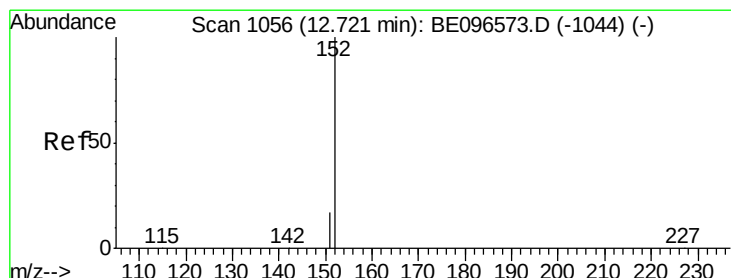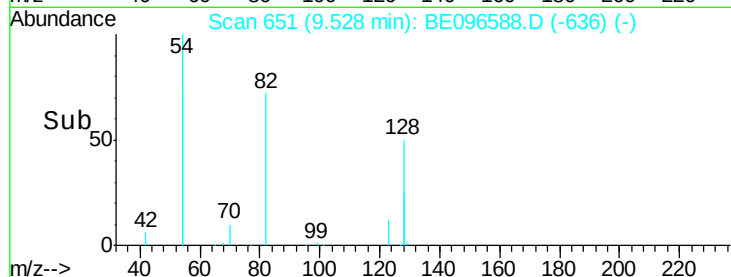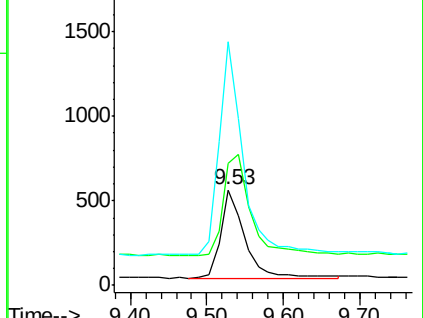

#11

2-Methylnaphthalene-d10

Concen: 0.330 ng

RT: 12.72 min Scan# 1056

Delta R.T. -0.00 min

Lab File: BE096588.D


Acq: 16 May 2018 9:16

Tgt Ion: 152 Resp: 1624

Ion Ratio Lower Upper



152 100


151 19.6 15.4 23.0

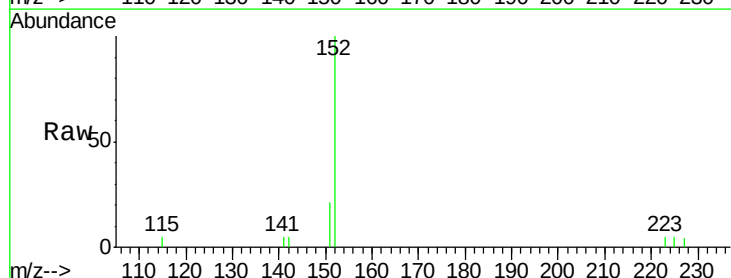

Abundance Ion 152.00 (151.70 to 152.70): BE096573.D (-1044) (-)

Ion 151.00 (150.70 to 151.70): BE096573.D (-1044) (-)

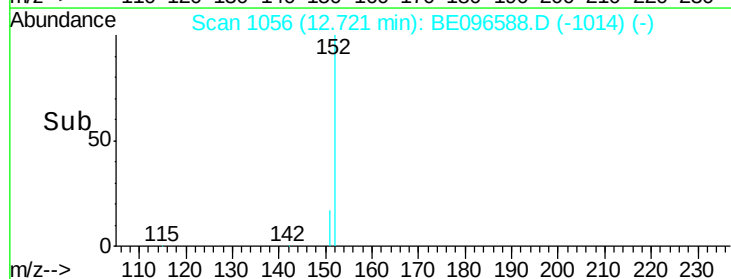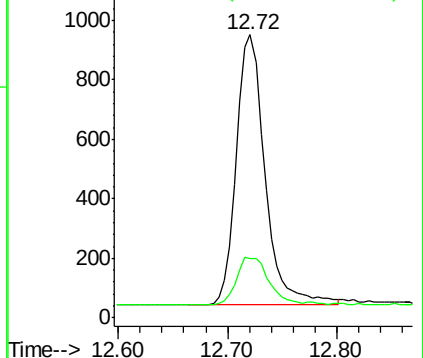

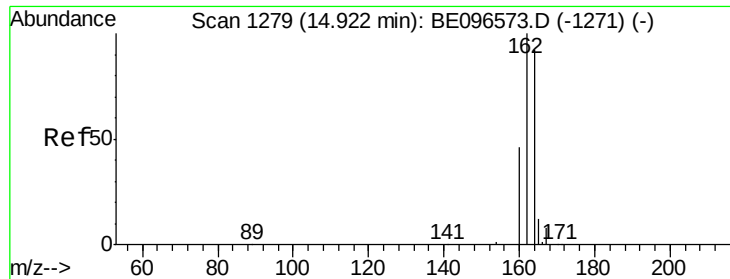

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.92 min Scan# 1279

Delta R.T. 0.00 min

Lab File: BE096588.D

Acq: 16 May 2018 9:16

Instrument :

BNA_E

ClientSampleId :

PB108420BL


Tgt Ion:164 Resp: 1537

Ion Ratio Lower Upper

164 100

162 111.2 83.1 124.7



160 50.7 37.1 55.7

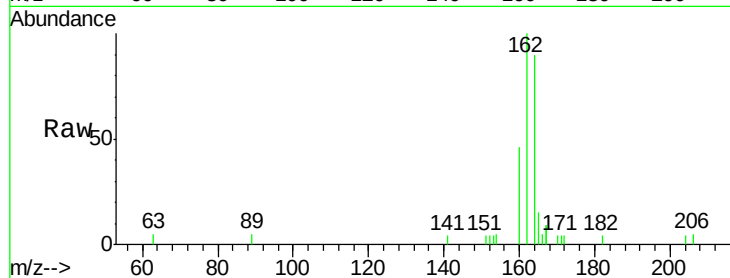


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

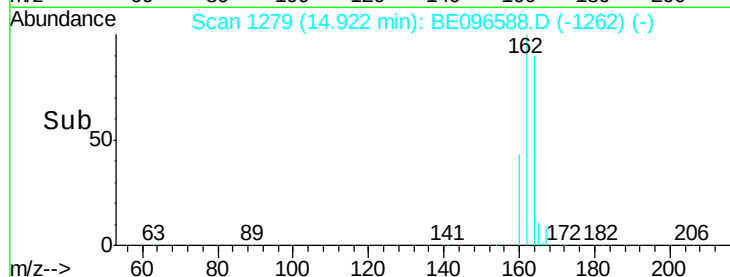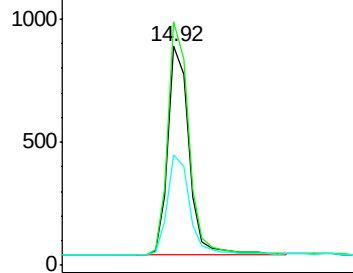

Time-->

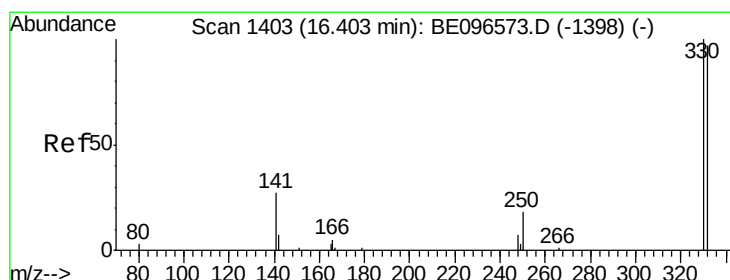

#14

2,4,6-Tribromophenol

Concen: 0.311 ng

RT: 16.40 min Scan# 1403

Delta R.T. 0.00 min

Lab File: BE096588.D

Acq: 16 May 2018 9:16


Tgt Ion:330 Resp: 189

Ion Ratio Lower Upper

330 100

332 93.1 152.7 229.1#



141 50.8 33.7 50.5#

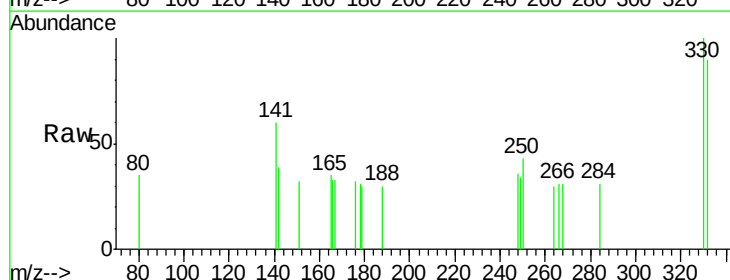


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

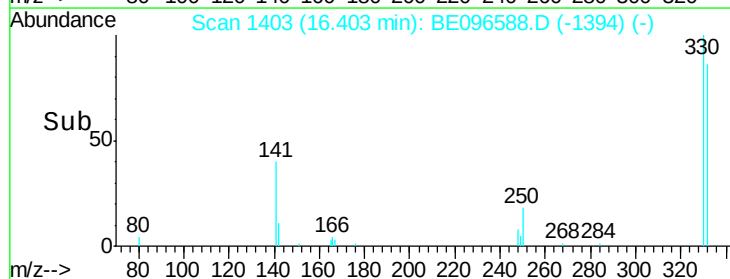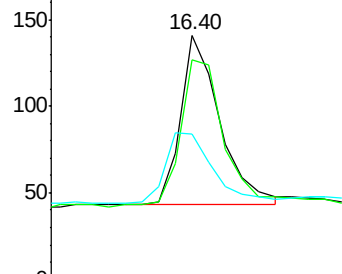

Time-->

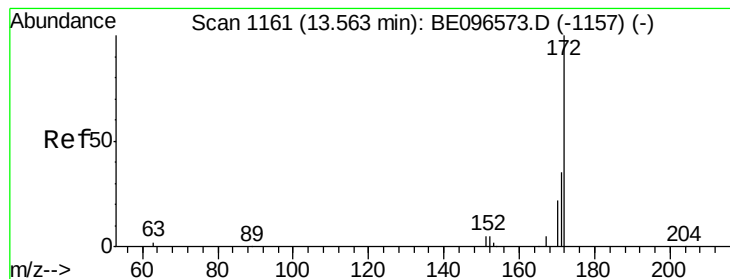

#15

2-Fluorobiphenyl

Concen: 0.364 ng

RT: 13.56 min Scan# 1161

Delta R.T. 0.00 min

Lab File: BE096588.D

Acq: 16 May 2018 9:16

Instrument :

BNA_E

ClientSampleId :

PB108420BL


Tgt Ion:172 Resp: 2403

Ion Ratio Lower Upper

172 100

171 37.3 29.9 44.9




170 24.7 21.8 32.8

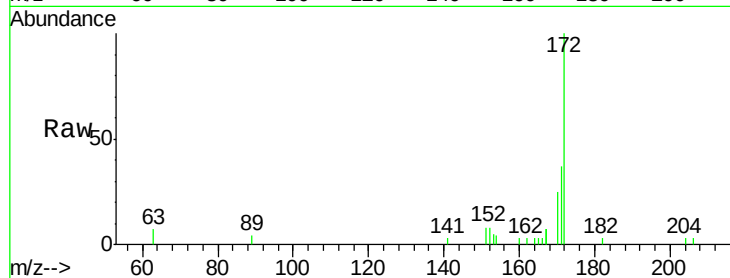

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

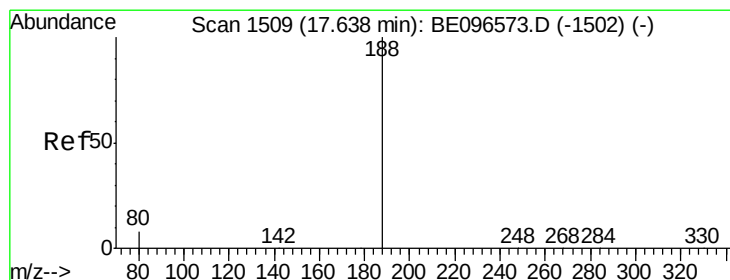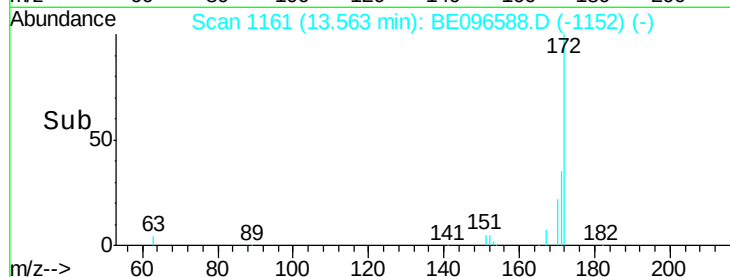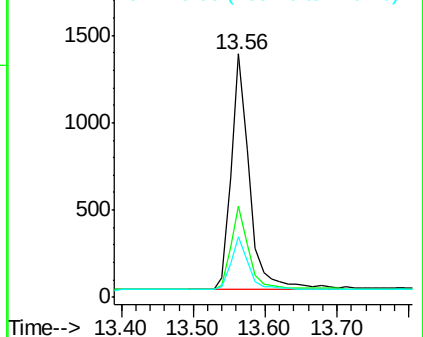

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.64 min Scan# 1509

Delta R.T. 0.00 min

Lab File: BE096588.D

Acq: 16 May 2018 9:16


Tgt Ion:188 Resp: 3468

Ion Ratio Lower Upper

188 100

94 0.0 3.9 5.9#



80 11.3 3.6 5.4#

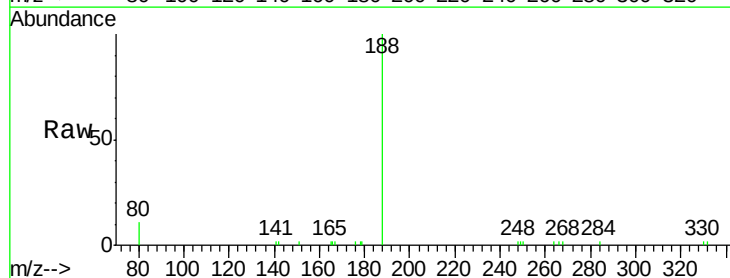


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

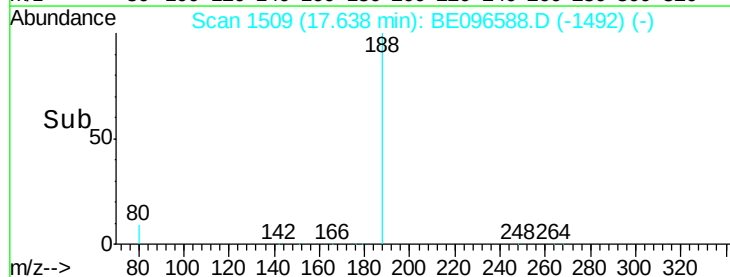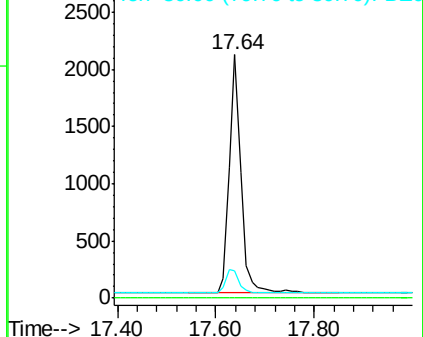

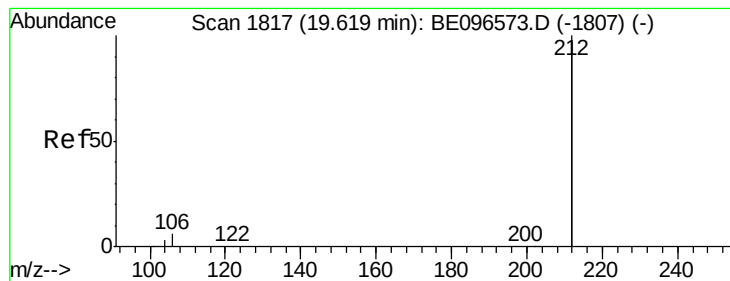

#25

Fluoranthene-d10

Concen: 0.371 ng

RT: 19.62 min Scan# 1818

Delta R.T. 0.01 min

Lab File: BE096588.D

Acq: 16 May 2018 9:16

Instrument :

BNA_E

ClientSampleId :

PB108420BL


Tgt Ion:212 Resp: 15747

Ion Ratio Lower Upper

212 100

106 2.7 2.8 4.2#




104 1.6 1.6 2.4

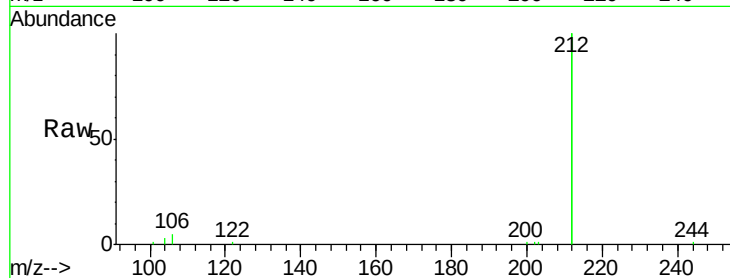

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

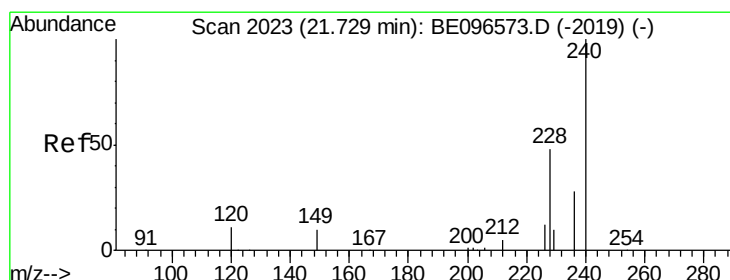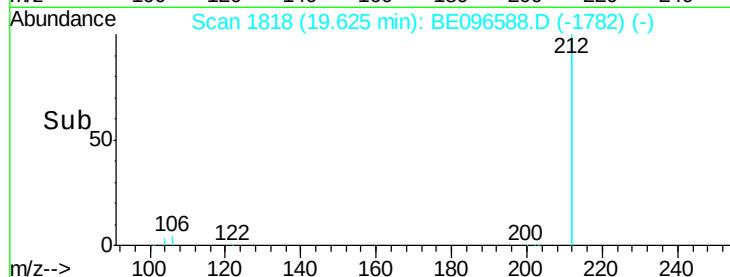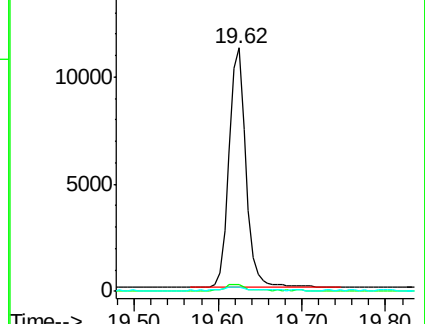

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.74 min Scan# 2024

Delta R.T. 0.01 min

Lab File: BE096588.D

Acq: 16 May 2018 9:16


Tgt Ion:240 Resp: 3687

Ion Ratio Lower Upper

240 100

120 7.3 5.5 8.3



236 27.3 20.7 31.1

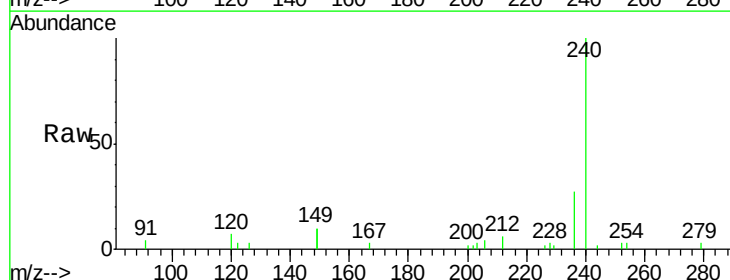


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

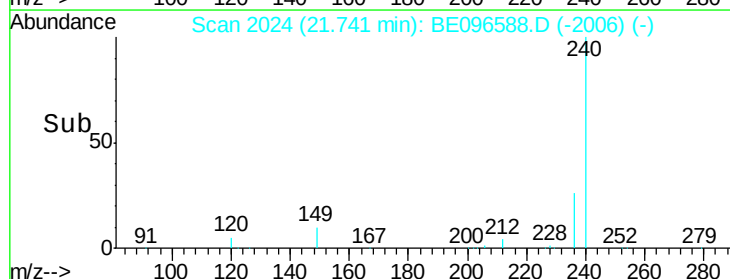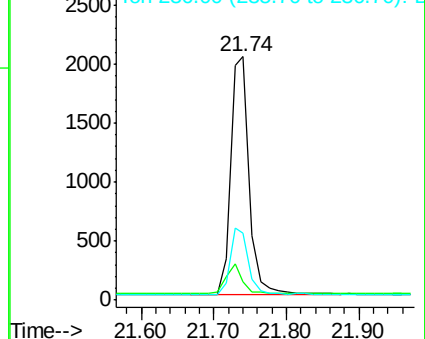

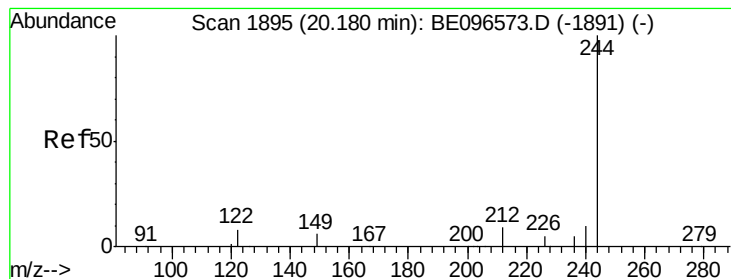

#29

Terphenyl-d14

Concen: 0.349 ng

RT: 20.18 min Scan# 1895

Delta R.T. 0.00 min

Lab File: BE096588.D

Acq: 16 May 2018 9:16

Instrument :

BNA_E

ClientSampleId :

PB108420BL


Tgt Ion:244 Resp: 2914

Ion Ratio Lower Upper

244 100

212 11.3 25.4 38.0#




122 9.4 8.1 12.1

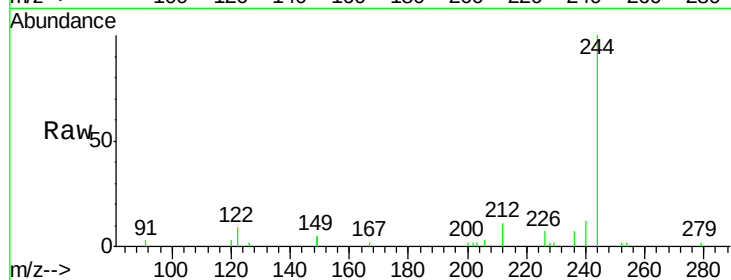

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

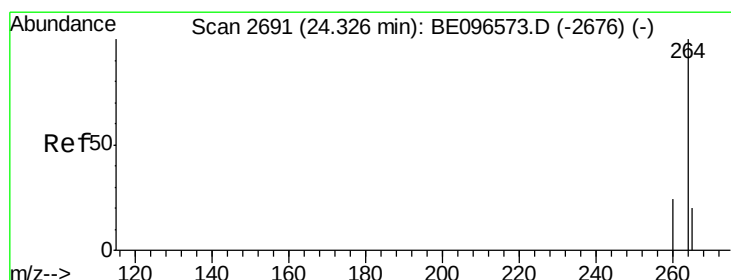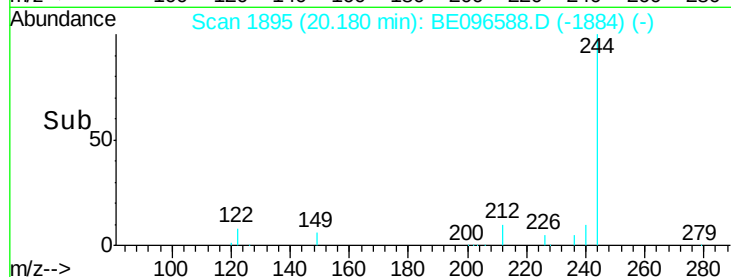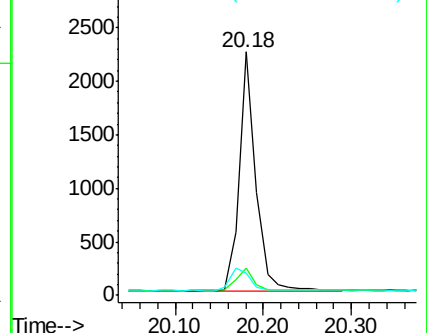

#34

Perylene-d12

Concen: 0.400 ng

RT: 24.33 min Scan# 2693

Delta R.T. 0.01 min

Lab File: BE096588.D

Acq: 16 May 2018 9:16


Tgt Ion:264 Resp: 3524

Ion Ratio Lower Upper

264 100

260 27.7 20.5 30.7

265 29.4 22.8 34.2

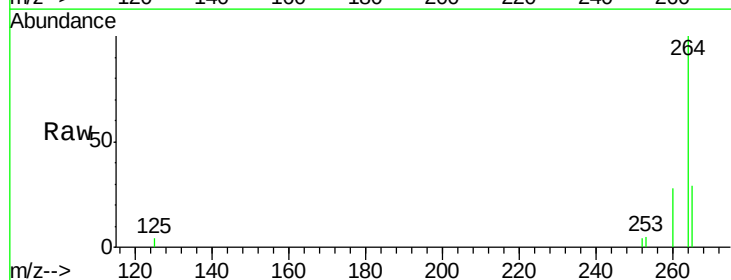

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

