


Data Path : Z:\HPCHEM1\BNA_E\Data\BE051618\
 Data File : BE096586.D
 Acq On : 16 May 2018 8:02
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 15 13:02:03 2018

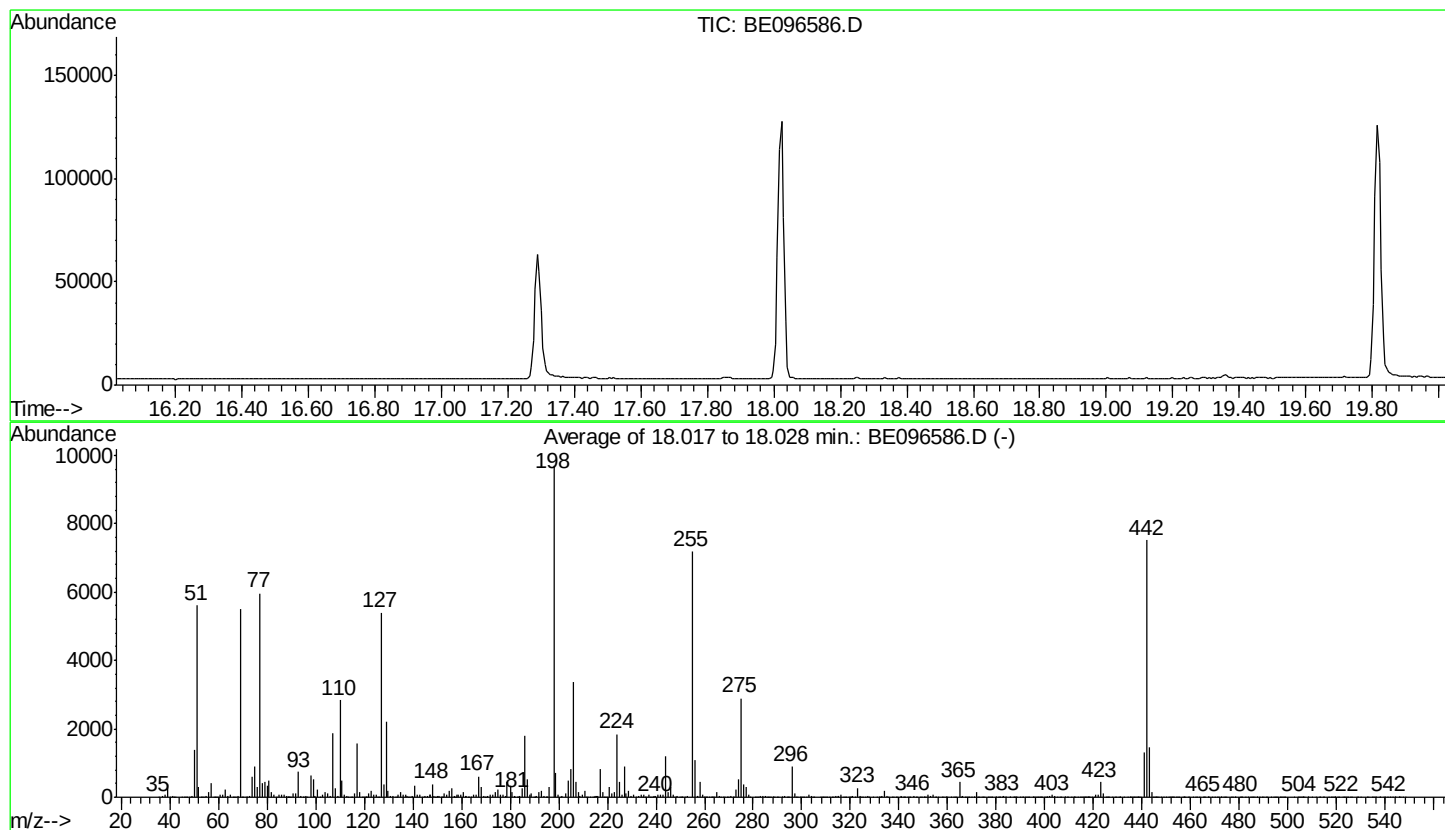

AutoFind: Scans 2626, 2627, 2628; Background Corrected with Scan 2619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.8	5601	PASS
68	69	0.00	2	0.7	38	PASS
69	198	0.00	100	56.7	5494	PASS
70	69	0.00	2	0.3	19	PASS
127	198	10	80	55.7	5400	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	9695	PASS
199	198	5	9	7.2	701	PASS
275	198	10	60	29.8	2886	PASS
365	198	1	100	4.6	447	PASS
441	443	0.01	100	88.4	1297	PASS
442	198	50	100	77.4	7508	PASS
443	442	15	24	19.6	1468	PASS