


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE051619\
Data File : BE099619.D
Acq On : 16 May 2019 10:49
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051419.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 14 19:30:50 2019

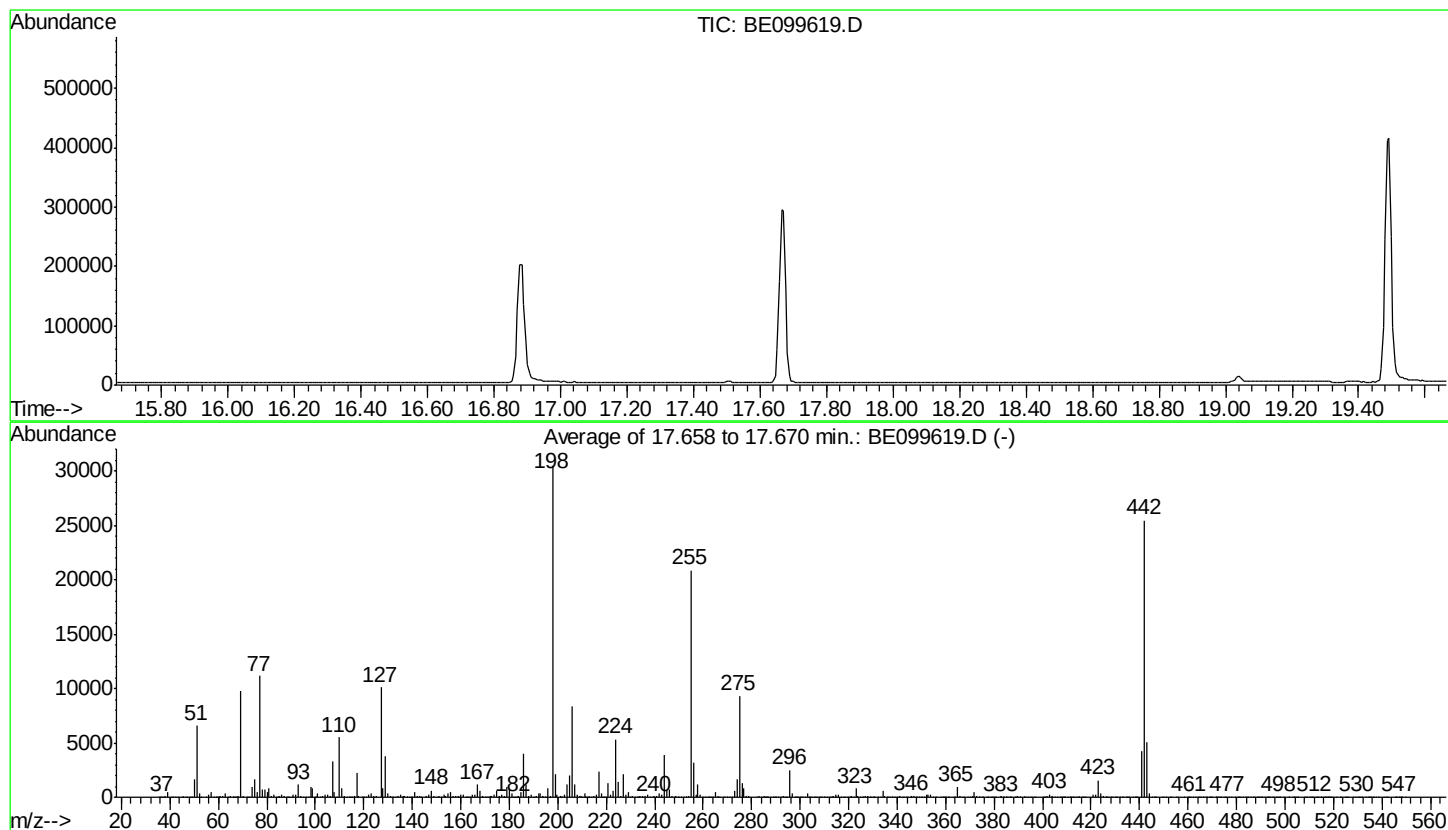

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.6	6585	PASS
68	69	0.00	2	0.7	71	PASS
69	198	0.00	100	32.1	9799	PASS
70	69	0.00	2	0.8	78	PASS
127	198	10	80	33.1	10100	PASS
197	198	0.00	2	0.4	123	PASS
198	198	100	100	100.0	30485	PASS
199	198	5	9	7.1	2176	PASS
275	198	10	60	30.6	9338	PASS
365	198	1	100	3.3	1003	PASS
441	198	0.01	100	13.8	4197	PASS
442	198	50	100	83.4	25436	PASS
443	442	15	24	20.0	5083	PASS