


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE051619\
 Data File : BE099634.D
 Acq On : 16 May 2019 22:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 14 19:30:50 2019

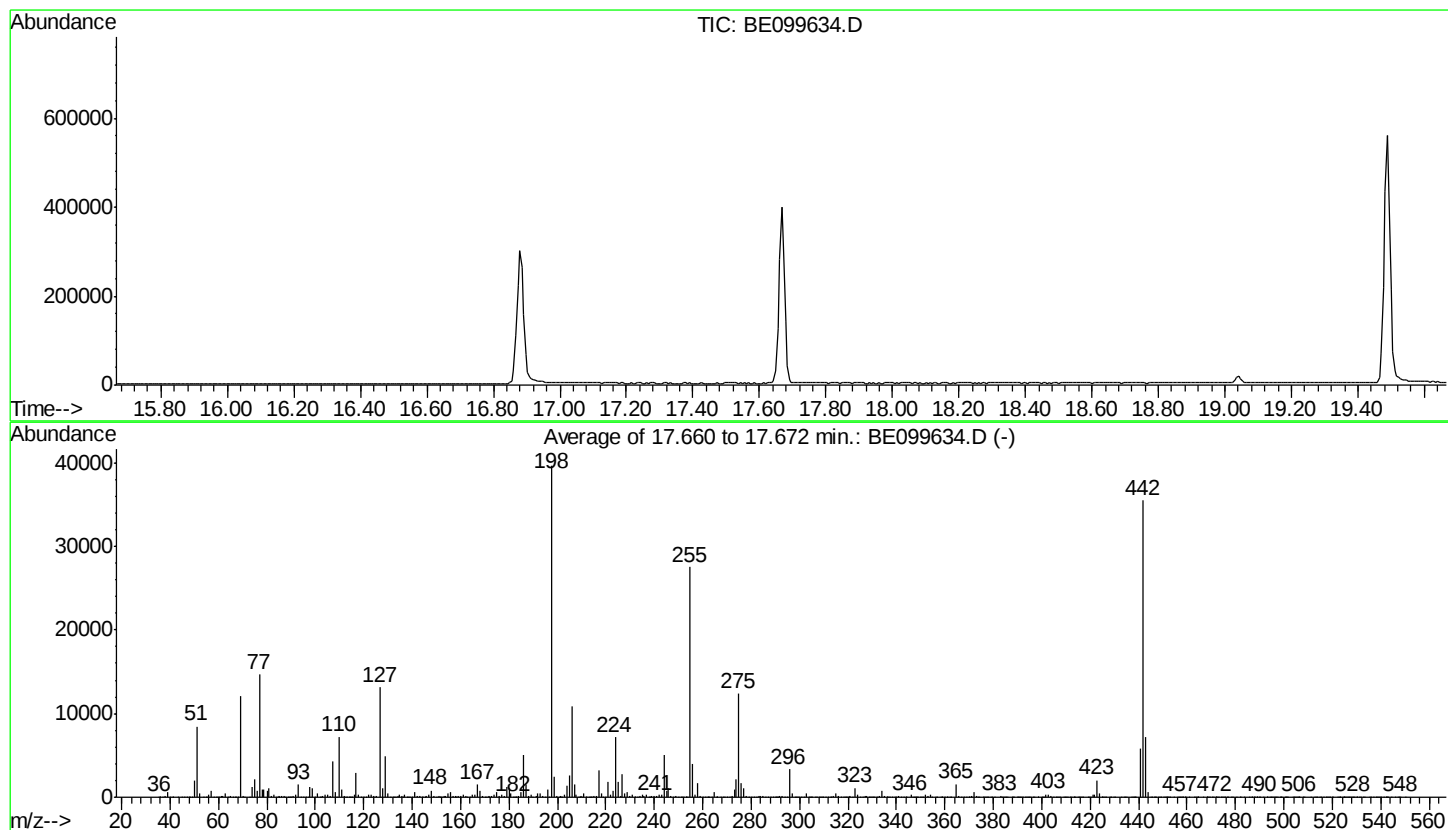

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.3	8427	PASS
68	69	0.00	2	0.2	21	PASS
69	198	0.00	100	30.6	12117	PASS
70	69	0.00	2	0.9	106	PASS
127	198	10	80	33.2	13142	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39633	PASS
199	198	5	9	6.3	2508	PASS
275	198	10	60	31.2	12370	PASS
365	198	1	100	4.0	1593	PASS
441	198	0.01	100	14.7	5828	PASS
442	198	50	100	89.5	35474	PASS
443	442	15	24	20.2	7171	PASS