
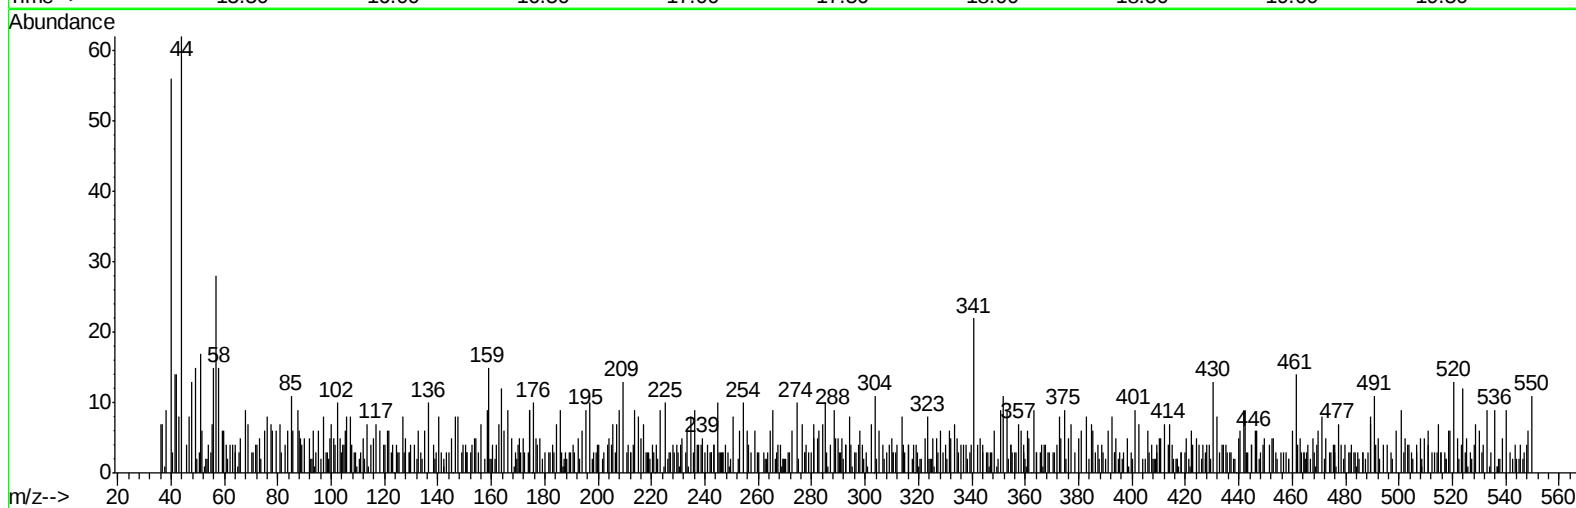


Data File : BE096599.D
Acq On : 17 May 2018 8:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 06:47:42 2018
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 17 16:15:19 2018
Response via : Initial Calibration

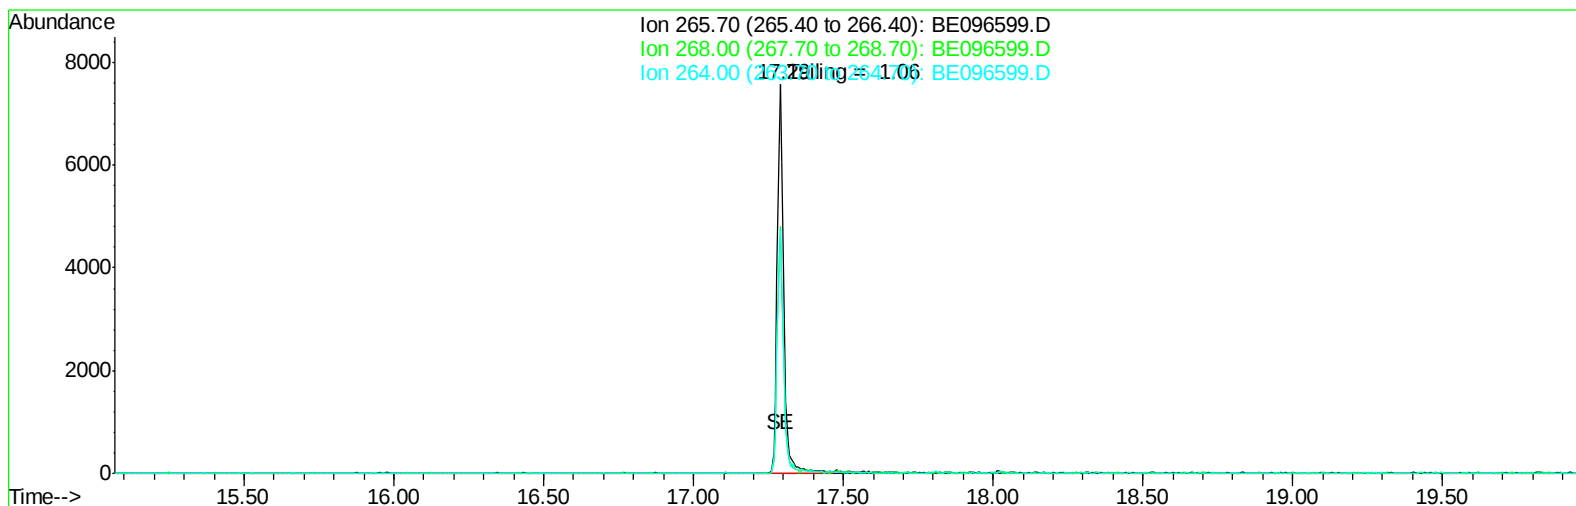

TIC: BE096599.D



(69) Pentachlorophenol (C)
11.109min (-0.006) 130.35ng

response 6

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	36.36#
264.00	61.90	54.55
0.00	0.00	0.00

Data File : BE096599.D
Acq On : 17 May 2018 8:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 06:47:42 2018
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF051018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 17 16:15:19 2018
Response via : Initial Calibration

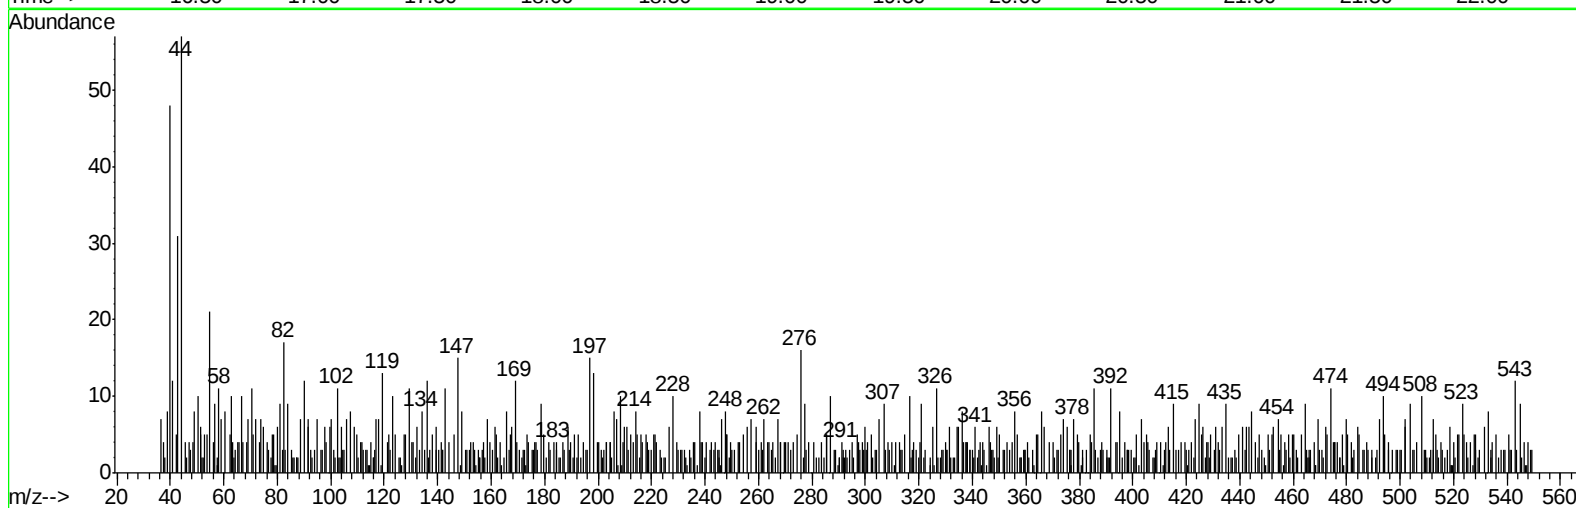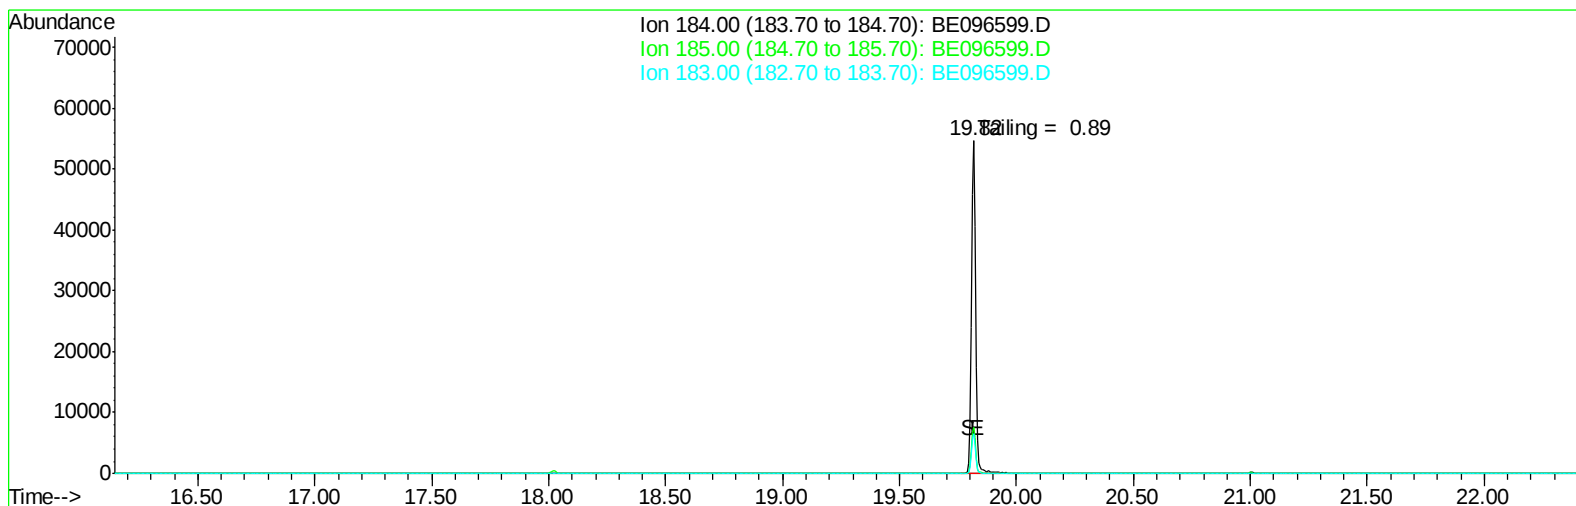

TIC: BE096599.D

(76) Benzidine

12.643min (-0.014) 18.08ng

response 8

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	28.57#
183.00	11.60	57.14#
0.00	0.00	0.00