


Data Path : Z:\HPCHEM1\BNA_E\Data\BE051718\
 Data File : BE096599.D
 Acq On : 17 May 2018 8:23
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 15 13:02:03 2018

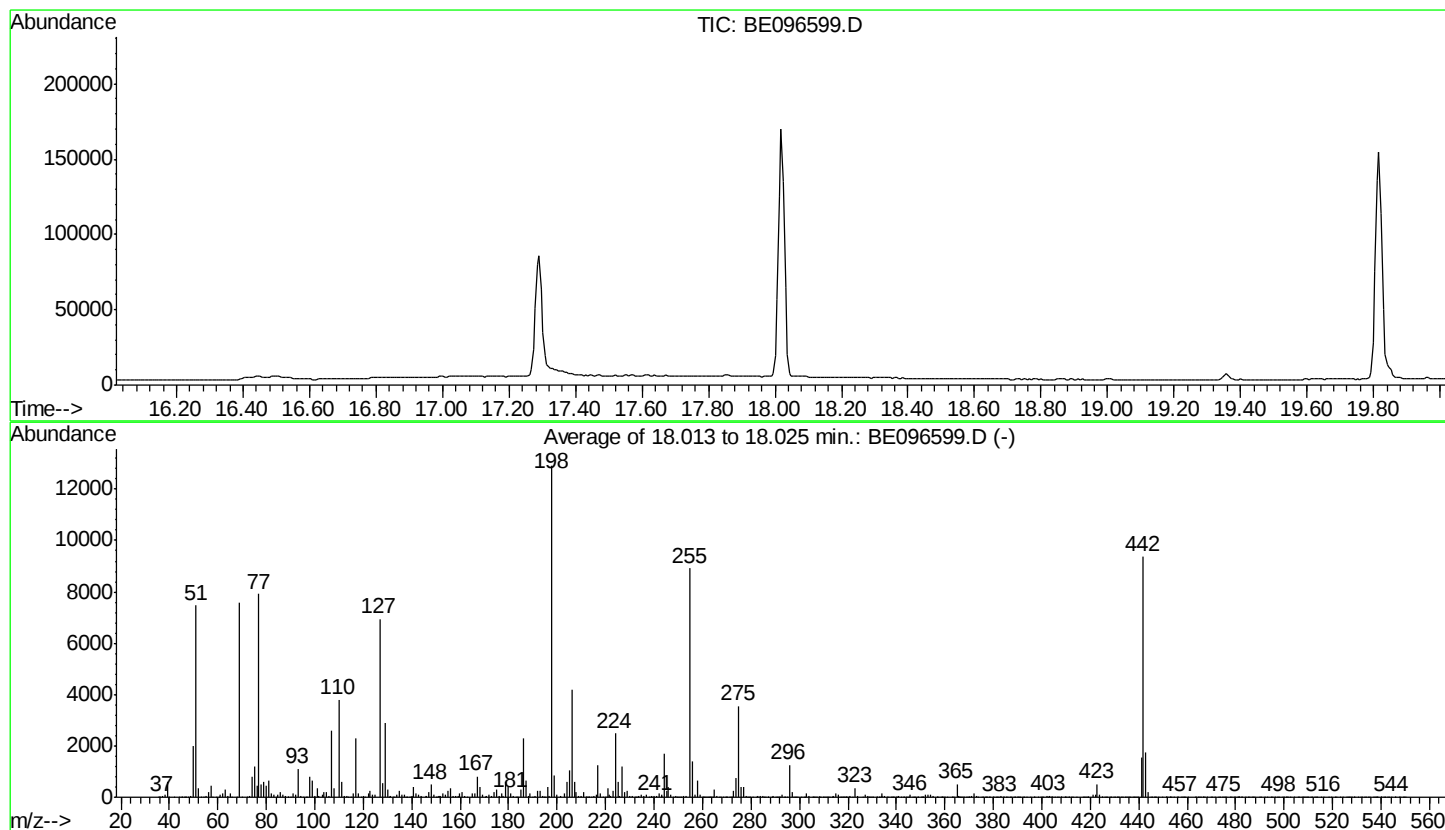

AutoFind: Scans 2625, 2626, 2627; Background Corrected with Scan 2615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.7	7457	PASS
68	69	0.00	2	0.2	18	PASS
69	198	0.00	100	58.6	7564	PASS
70	69	0.00	2	0.3	26	PASS
127	198	10	80	53.8	6944	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12915	PASS
199	198	5	9	6.4	825	PASS
275	198	10	60	27.6	3564	PASS
365	198	1	100	4.0	515	PASS
441	443	0.01	100	89.1	1549	PASS
442	198	50	100	72.4	9353	PASS
443	442	15	24	18.6	1738	PASS