


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE052019\
Data File : BE099657.D
Acq On : 20 May 2019 9:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE052019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 20 19:29:40 2019

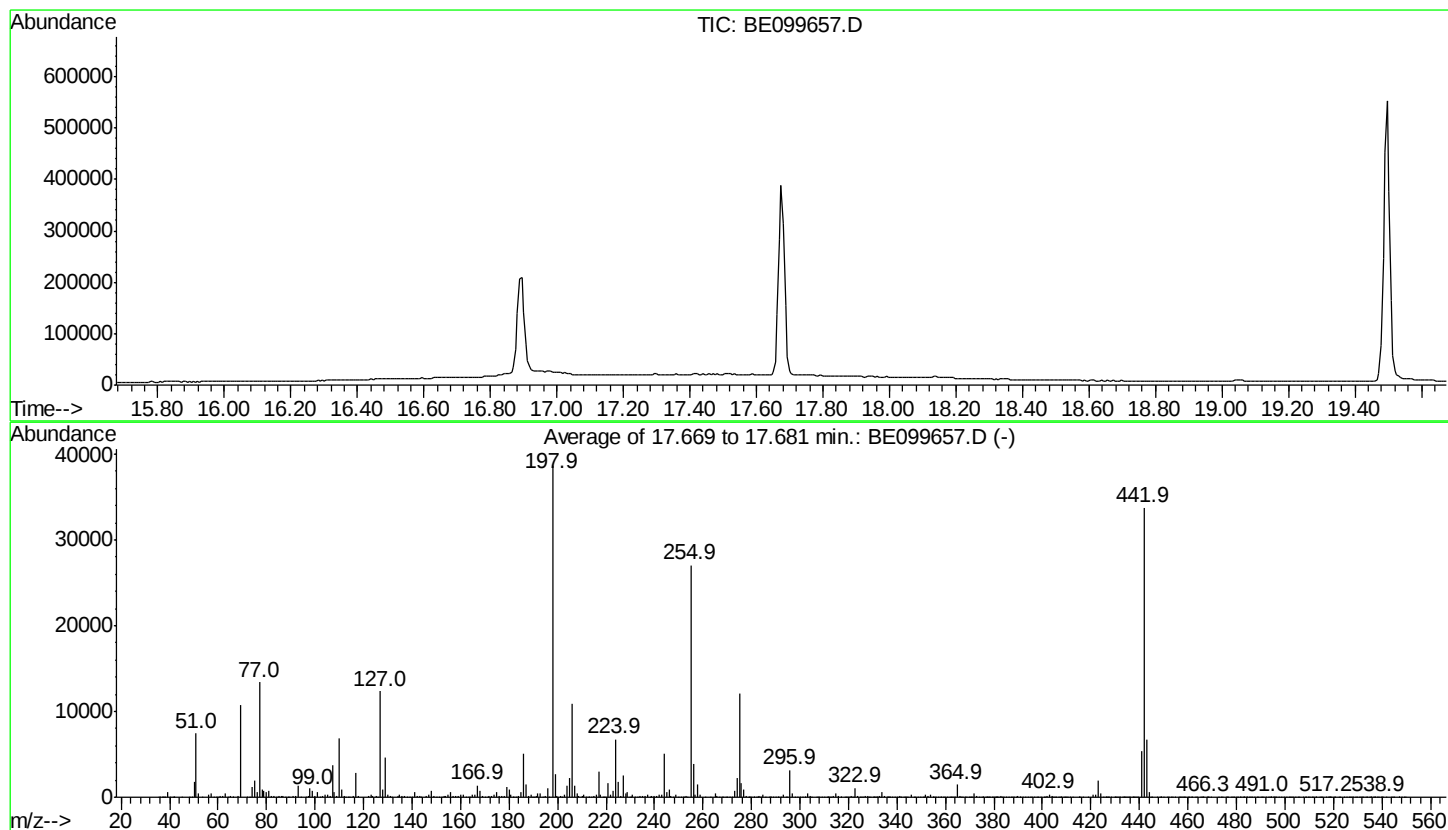

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.2	7416	PASS
68	69	0.00	2	1.6	167	PASS
69	198	0.00	100	27.6	10683	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.0	12365	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38662	PASS
199	198	5	9	6.8	2631	PASS
275	198	10	60	31.2	12058	PASS
365	198	1	100	3.8	1484	PASS
441	198	0.01	100	13.9	5389	PASS
442	198	50	100	87.3	33749	PASS
443	442	15	24	19.8	6692	PASS