


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE052019\
 Data File : BE099667.D
 Acq On : 20 May 2019 19:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE052019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 20 19:29:40 2019

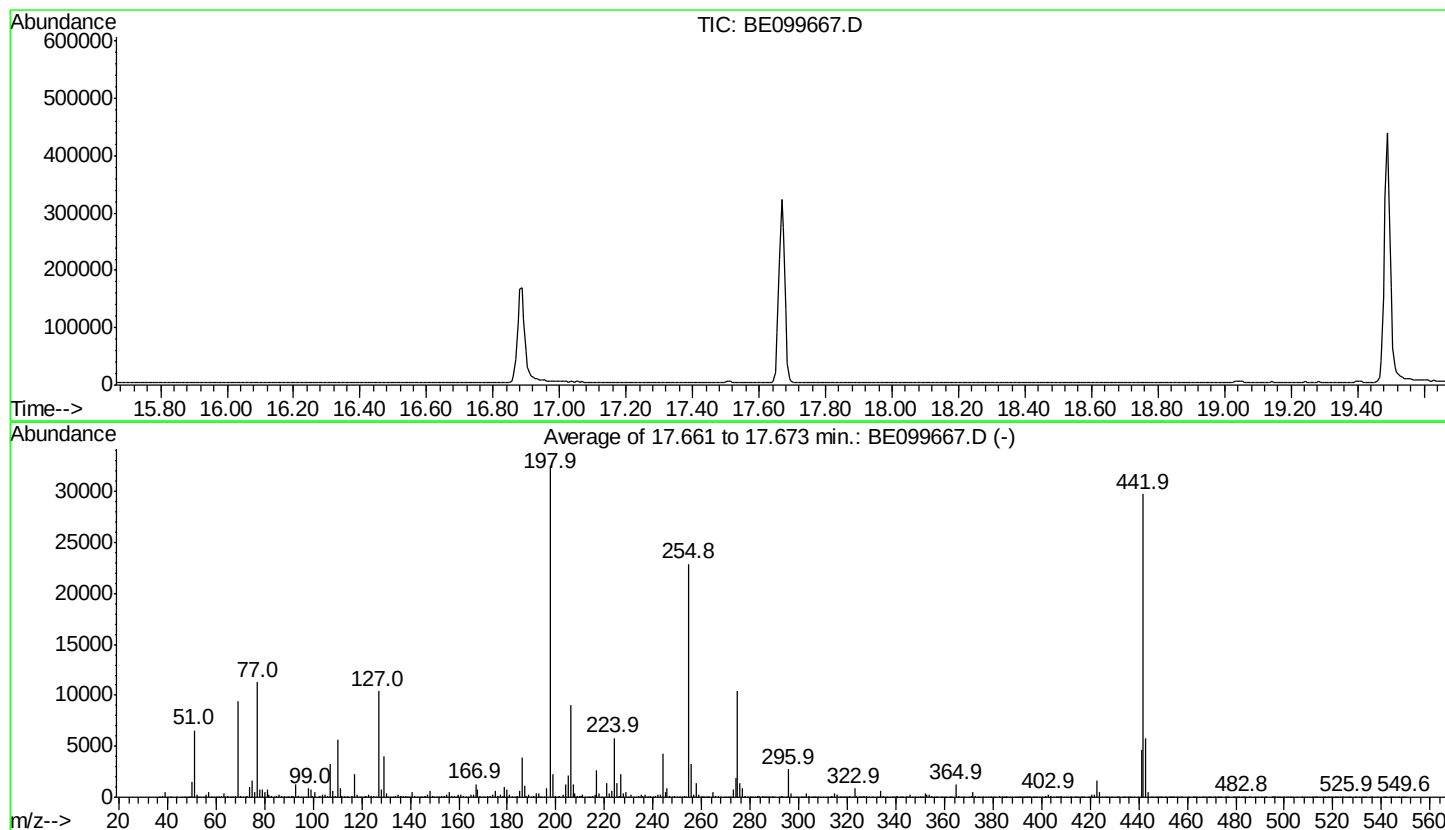

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.2	6584	PASS
68	69	0.00	2	1.5	138	PASS
69	198	0.00	100	29.0	9434	PASS
70	69	0.00	2	0.8	72	PASS
127	198	10	80	31.9	10387	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	32542	PASS
199	198	5	9	6.9	2253	PASS
275	198	10	60	32.1	10448	PASS
365	198	1	100	3.8	1247	PASS
441	198	0.01	100	14.2	4635	PASS
442	198	50	100	91.3	29715	PASS
443	442	15	24	19.6	5825	PASS