

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE052119\
 Data File : BE099696.D
 Acq On : 21 May 2019 19:22
 Operator : JU/SJ
 Sample : PB119824BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB119824BL

Quant Time: May 22 08:26:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE052019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 20 19:29:40 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	1533	0.40	ng	0.00
7) Naphthalene-d8	10.61	136	4902	0.40	ng	0.00
13) Acenaphthene-d10	14.49	164	3407	0.40	ng	0.00
19) Phenanthrene-d10	17.23	188	9668	0.40	ng	0.00
27) Chrysene-d12	21.41	240	14802	0.40	ng	0.00
34) Perylene-d12	23.96	264	18091	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.38	112	1495	0.39	ng	0.00
5) Phenol-d6	6.98	99	1932	0.38	ng	0.00
8) Nitrobenzene-d5	8.98	82	1366	0.32	ng	0.00
11) 2-Methylnaphthalene-d10	12.22	152	3249	0.38	ng	0.00
14) 2,4,6-Tribromophenol	16.01	330	407	0.29	ng	0.03
15) 2-Fluorobiphenyl	13.12	172	4941	0.38	ng	0.01
25) Fluoranthene-d10	19.27	212	54415	0.41	ng	0.00
29) Terphenyl-d14	19.86	244	11348	0.43	ng	0.00


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE052119\
Data File : BE099696.D
Acq On : 21 May 2019 19:22
Operator : JU/SJ
Sample : PB119824BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB119824BL

Quant Time: May 22 08:26:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE052019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 20 19:29:40 2019
Response via : Initial Calibration

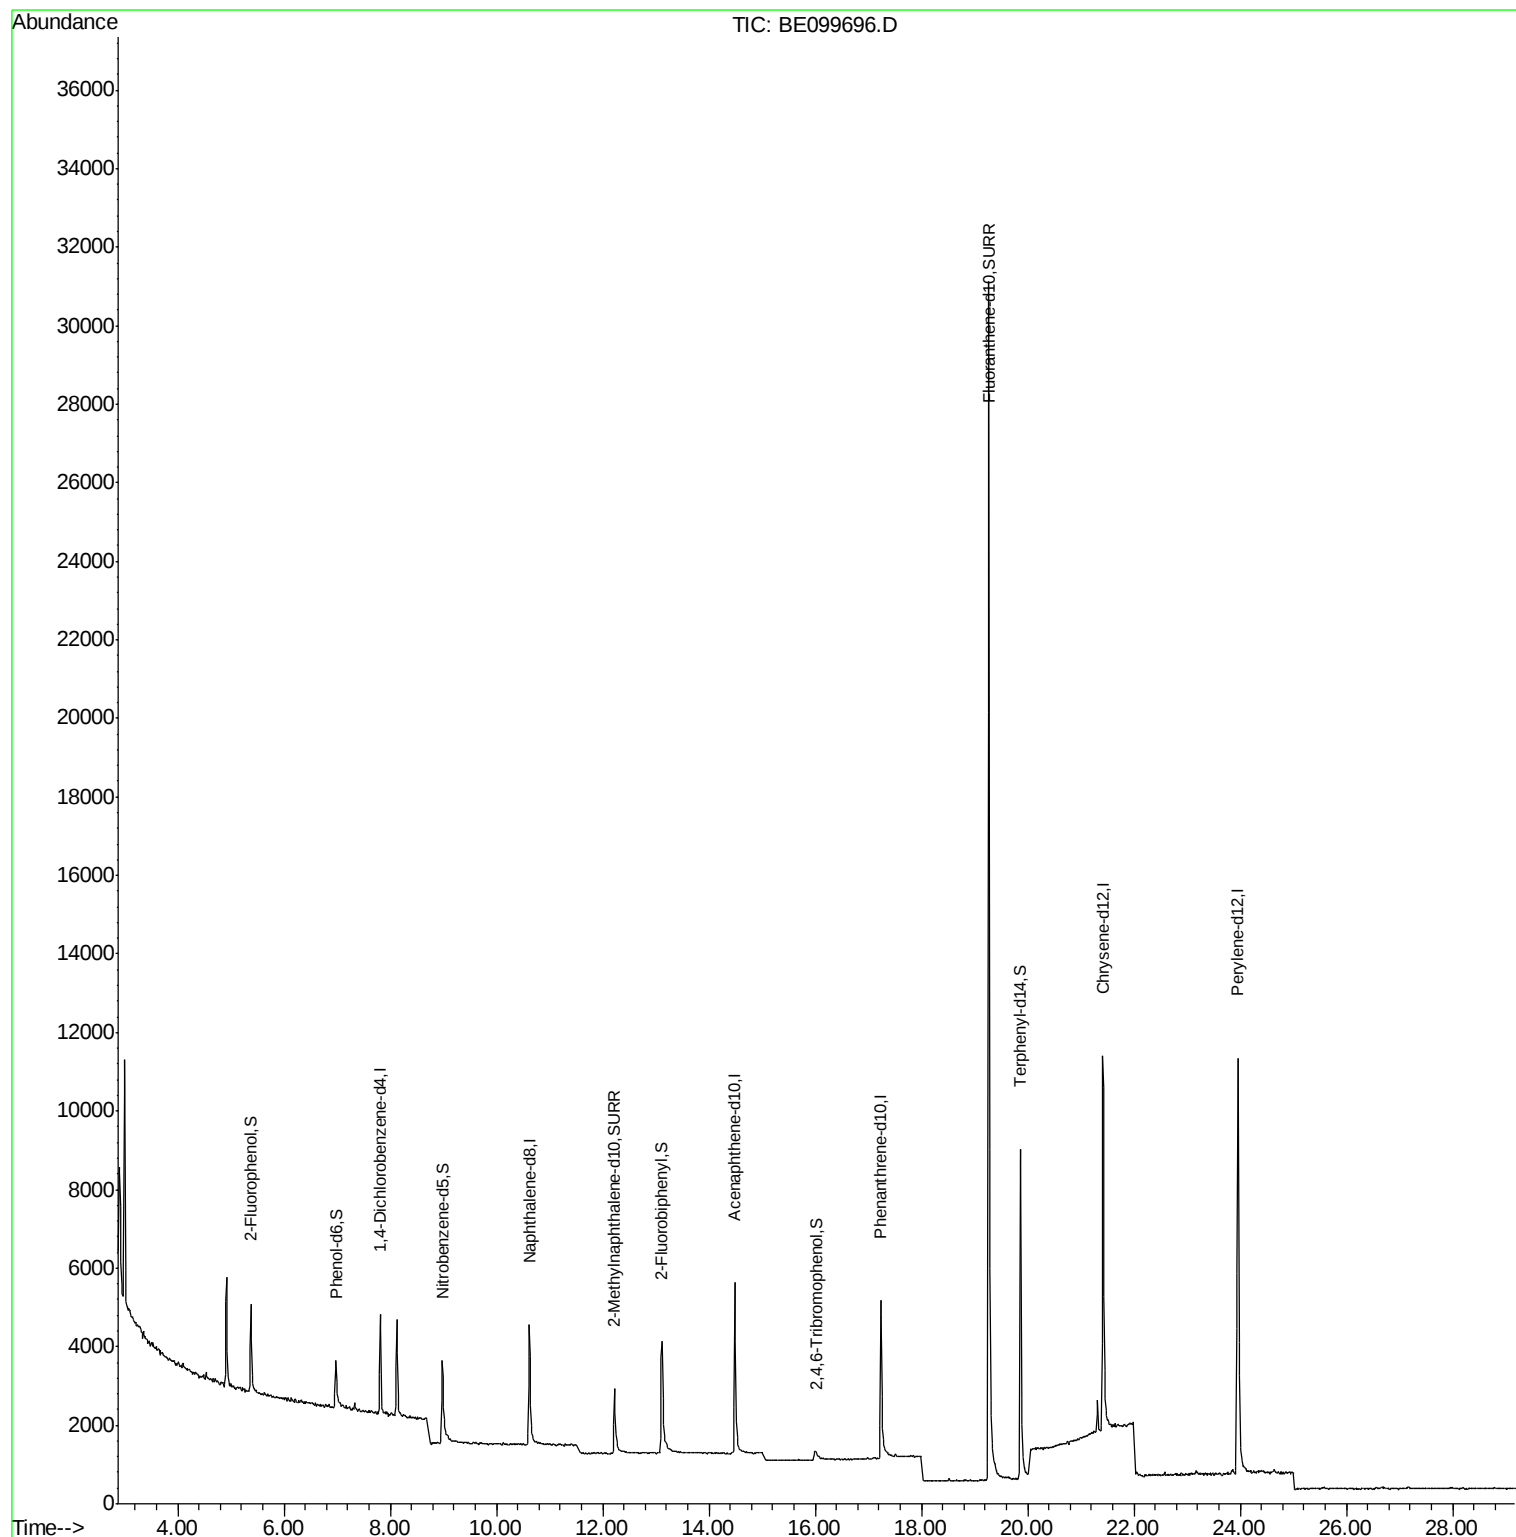



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.81 min Scan# 429

Delta R.T. -0.01 min

Lab File: BE099696.D

Acq: 21 May 2019 19:22

Instrument :

BNA_E

ClientSampleId :

PB119824BL


Tot Ion:152 Resp: 1533

Ion Ratio Lower Upper

152 100

150 145.0 109.2 163.8




115 64.1 43.7 65.5

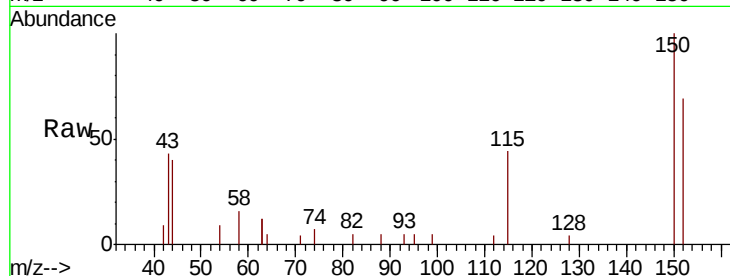

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

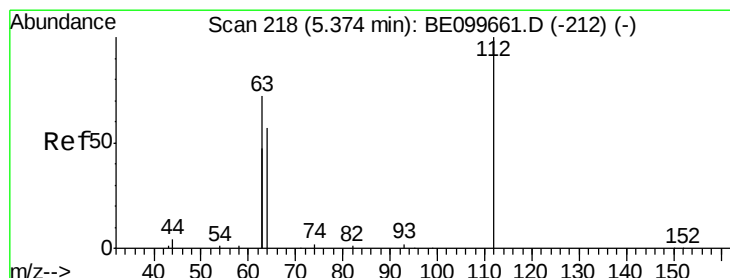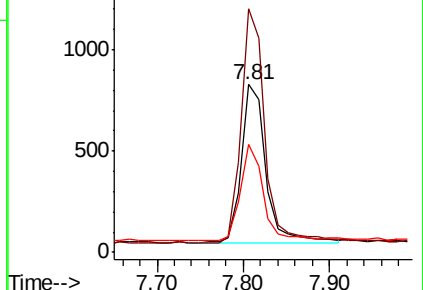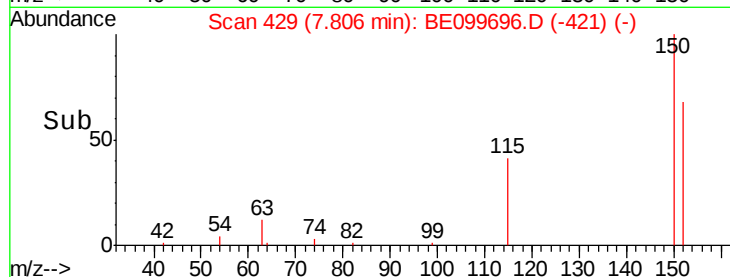

#4

2-Fluorophenol

Concen: 0.386 ng

RT: 5.38 min Scan# 218

Delta R.T. 0.00 min

Lab File: BE099696.D

Acq: 21 May 2019 19:22


Tgt Ion:112 Resp: 1495

Ion Ratio Lower Upper

112 100

64 54.8 43.4 65.2



63 118.9 96.9 145.3

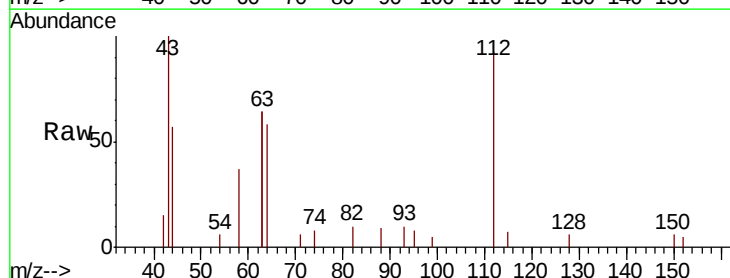


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

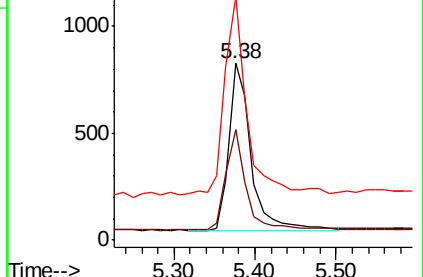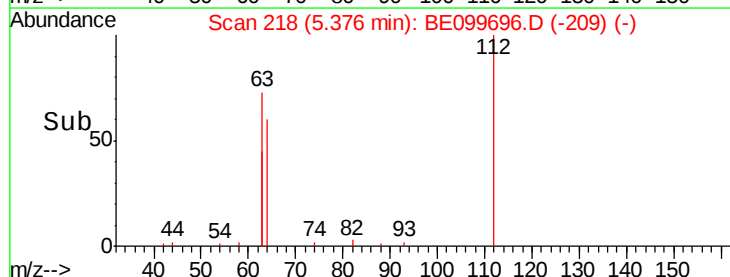

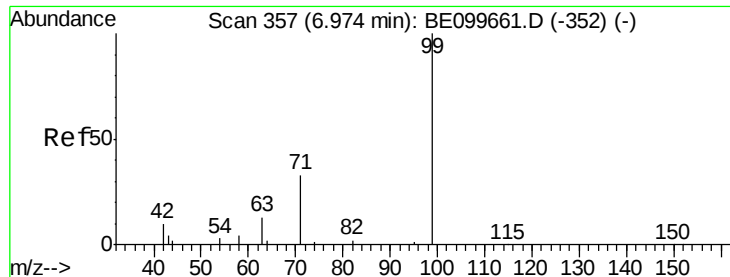

#5

Phenol-d6

Concen: 0.377 ng

RT: 6.98 min Scan# 357

Delta R.T. 0.00 min

Lab File: BE099696.D

Acq: 21 May 2019 19:22

Instrument :

BNA_E

ClientSampleId :

PB119824BL


Tot Ion: 99 Resp: 1932

Ion Ratio Lower Upper

99 100

42 14.9 12.2 18.2




71 38.0 28.9 43.3

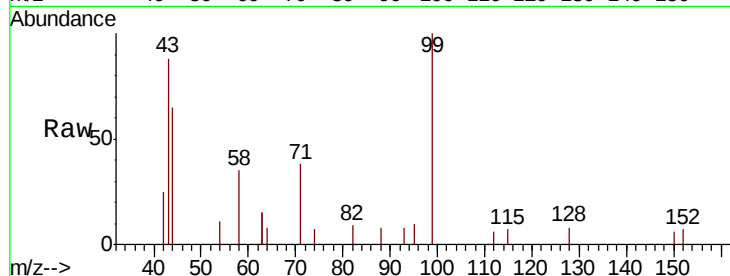

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

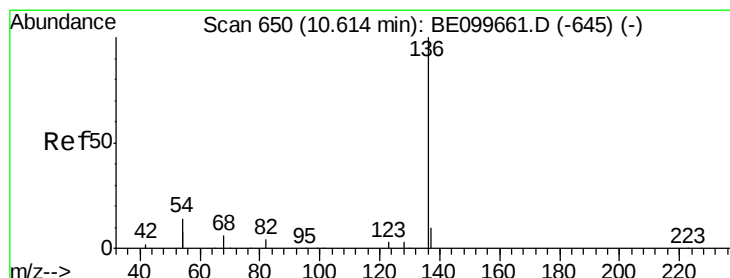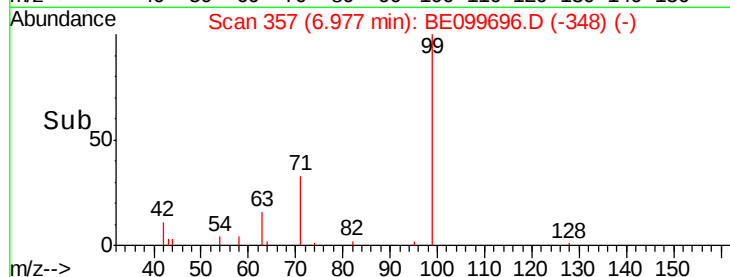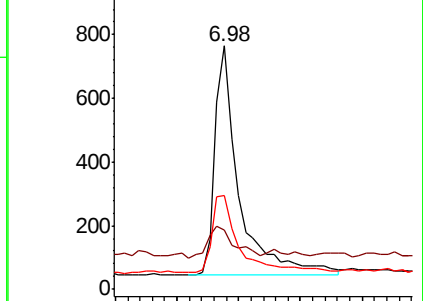

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.61 min Scan# 650

Delta R.T. 0.00 min

Lab File: BE099696.D

Acq: 21 May 2019 19:22

Tgt Ion: 136 Resp: 4902


Ion Ratio Lower Upper

136 100

137 12.0 9.0 13.6

54 32.9 22.3 33.5

68 9.2 6.0 9.0#


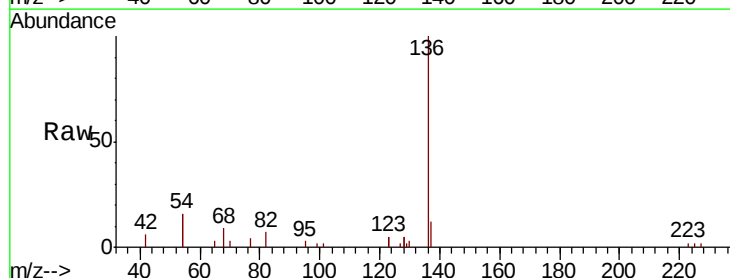


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

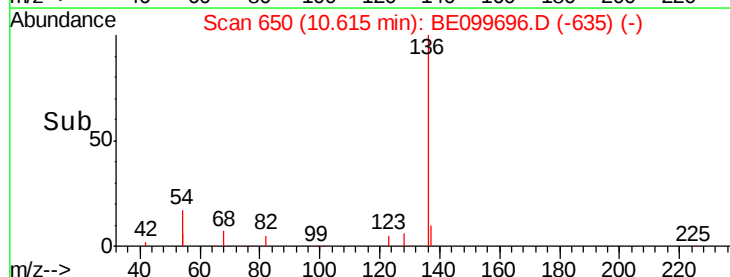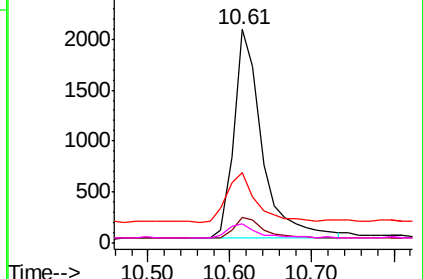



#8

Nitrobenzene-d5

Concen: 0.322 ng

RT: 8.98 min Scan# 524

Delta R.T. 0.00 min

Lab File: BE099696.D

Acq: 21 May 2019 19:22

Instrument :

BNA_E

ClientSampleId :

PB119824BL


Tot Ion: 82 Resp: 1366

Ion Ratio Lower Upper




82 100

128 150.0 117.7 176.5

54 151.6 106.6 160.0

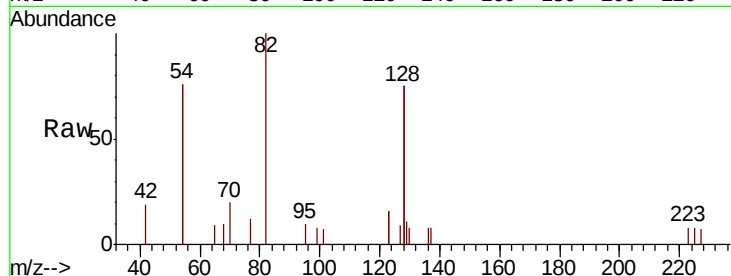

Abundance Ion 82.00 (81.70 to 82.70): BE0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BE0

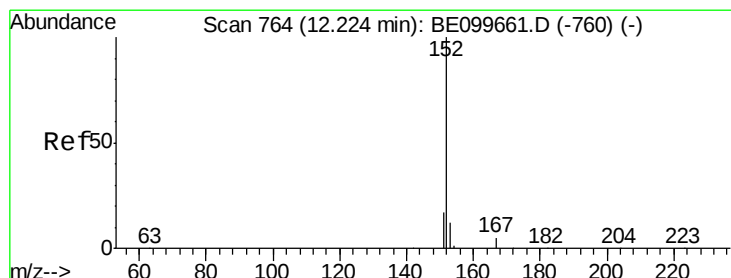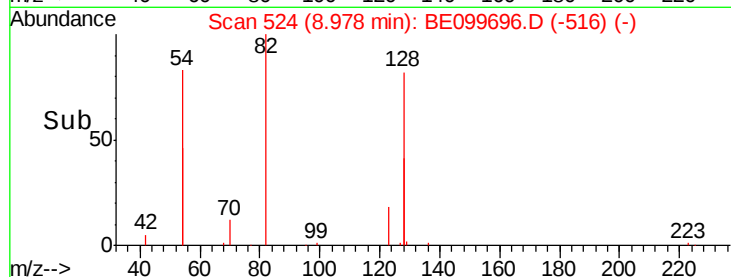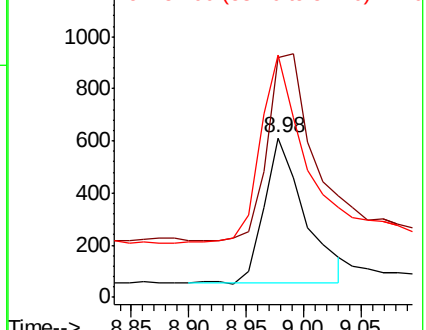

#11

2-Methylnaphthalene-d10

Concen: 0.384 ng

RT: 12.22 min Scan# 764

Delta R.T. -0.00 min

Lab File: BE099696.D


Acq: 21 May 2019 19:22

Tgt Ion: 152 Resp: 3249



Ion Ratio Lower Upper


152 100

151 19.8 15.0 22.4

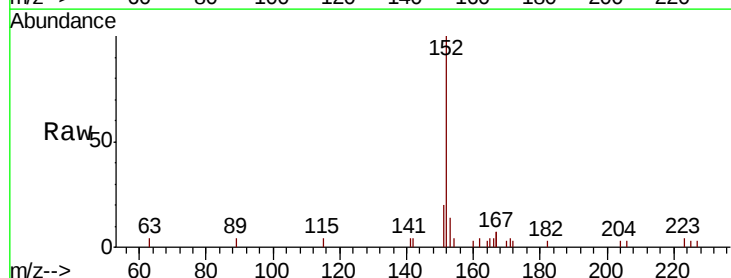

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E

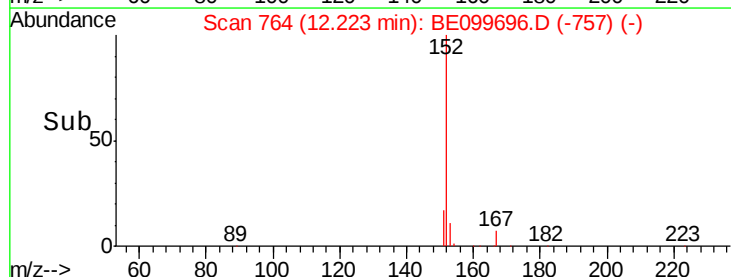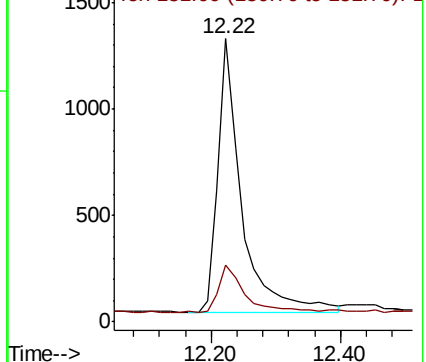


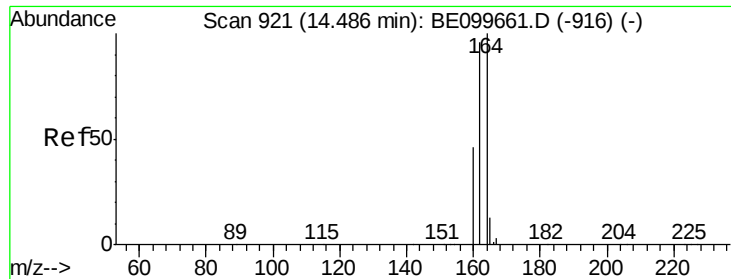




#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.49 min Scan# 921
 Delta R.T. -0.00 min
 Lab File: BE099696.D
 Acq: 21 May 2019 19:22

Instrument :
 BNA_E
 ClientSampleId :
 PB119824BL

Tot Ion:164 Resp: 3407
 Ion Ratio Lower Upper
 164 100
 162 104.9 76.5 114.7
 160 50.2 37.4 56.2

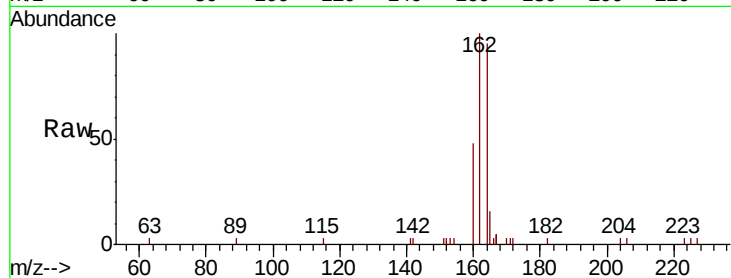


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

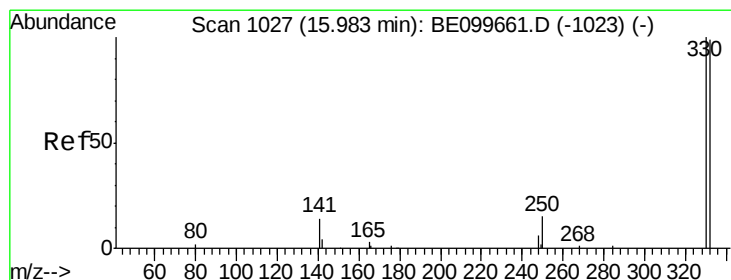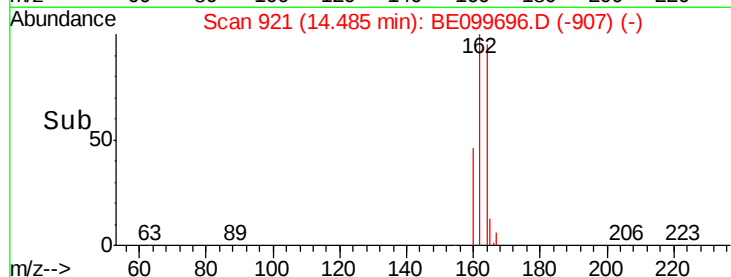
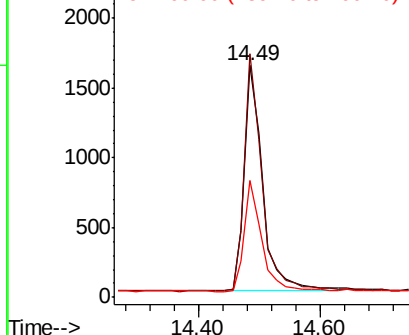



#14
 2,4,6-Tribromophenol
 Concen: 0.293 ng
 RT: 16.01 min Scan# 1029
 Delta R.T. 0.03 min
 Lab File: BE099696.D
 Acq: 21 May 2019 19:22

Tgt Ion:330 Resp: 407
 Ion Ratio Lower Upper
 330 100
 332 107.4 77.3 115.9
 141 0.0 18.9 28.3#

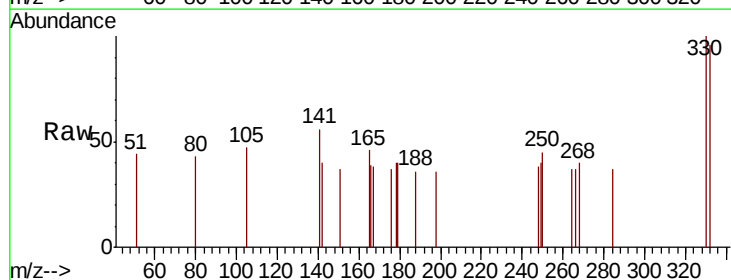

Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

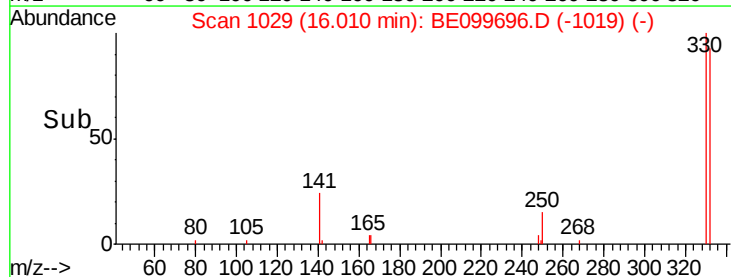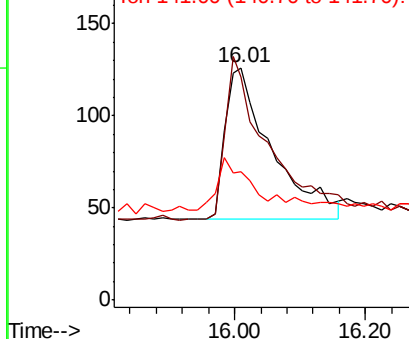

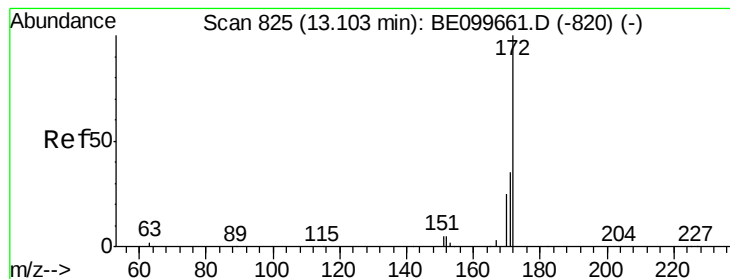

#15

2-Fluorobiphenyl

Concen: 0.382 ng

RT: 13.12 min Scan# 826

Delta R.T. 0.01 min

Lab File: BE099696.D

Acq: 21 May 2019 19:22

Instrument :

BNA_E

ClientSampleId :

PB119824BL


Tot Ion:172 Resp: 4941

Ion Ratio Lower Upper

172 100

171 34.7 28.7 43.1




170 24.7 20.9 31.3

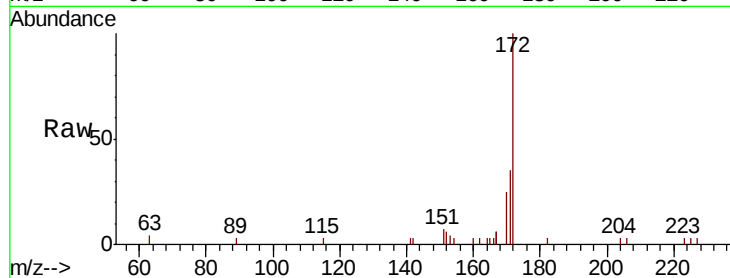

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

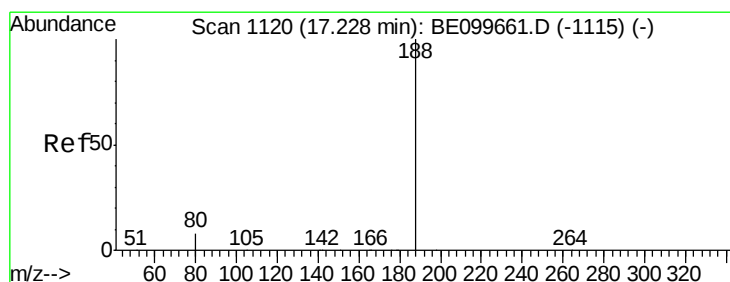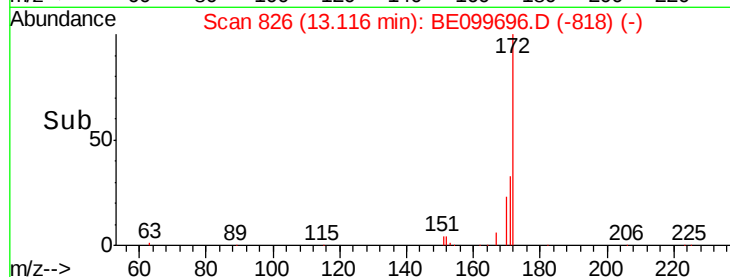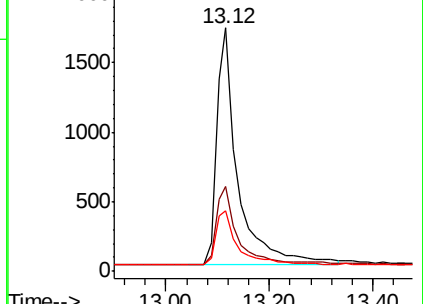

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.23 min Scan# 1120

Delta R.T. 0.00 min

Lab File: BE099696.D

Acq: 21 May 2019 19:22


Tgt Ion:188 Resp: 9668

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0



80 9.6 6.7 10.1

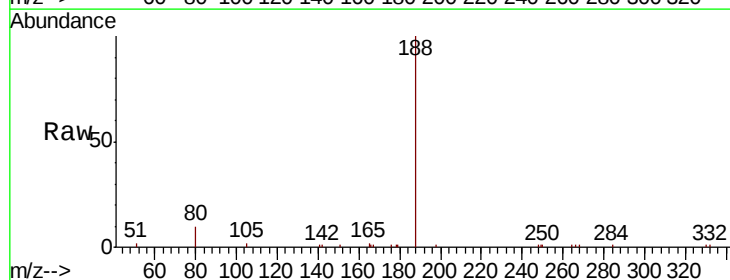


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

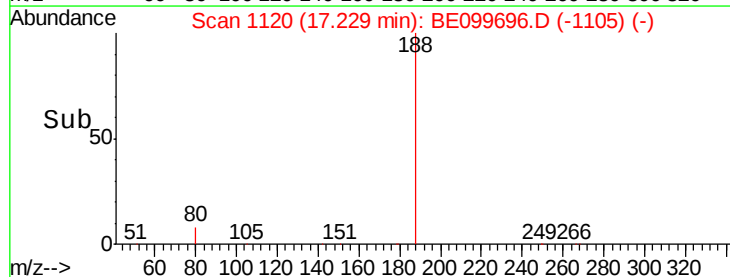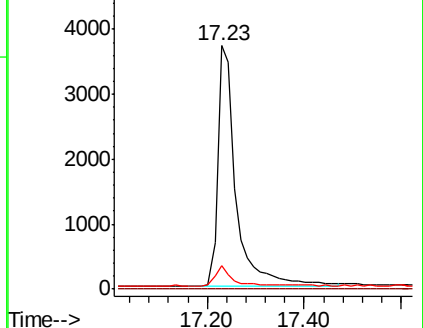

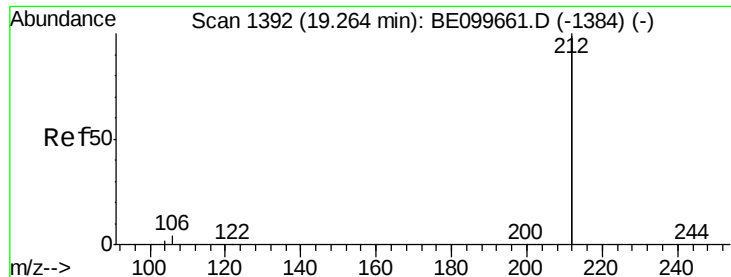

#25

Fluoranthene-d10

Concen: 0.412 ng

RT: 19.27 min Scan# 1393

Delta R.T. 0.01 min

Lab File: BE099696.D

Acq: 21 May 2019 19:22

Instrument :

BNA_E

ClientSampleId :

PB119824BL


Tot Ion:212 Resp: 54415

Ion Ratio Lower Upper

212 100

106 1.8 1.4 2.2




104 1.0 0.8 1.2

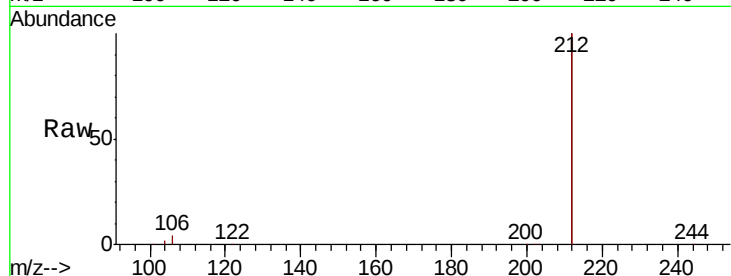

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

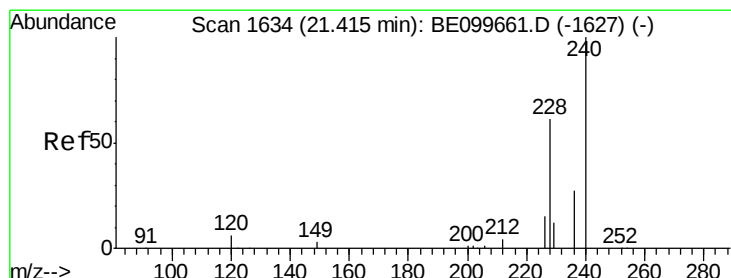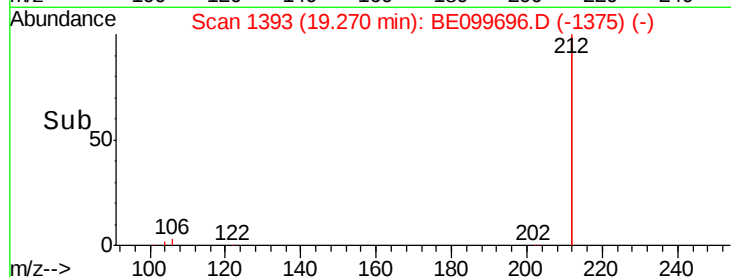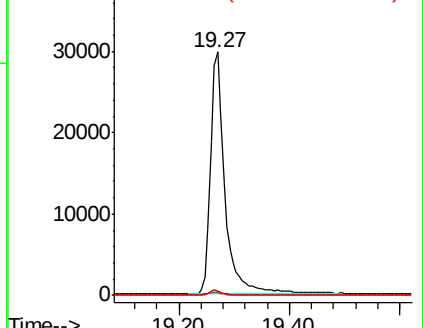

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.41 min Scan# 1634

Delta R.T. -0.00 min

Lab File: BE099696.D

Acq: 21 May 2019 19:22


Tgt Ion:240 Resp: 14802

Ion Ratio Lower Upper

240 100

120 7.9 5.4 8.0



236 29.1 21.7 32.5

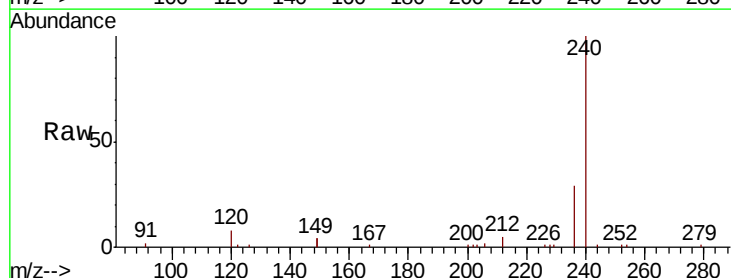


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

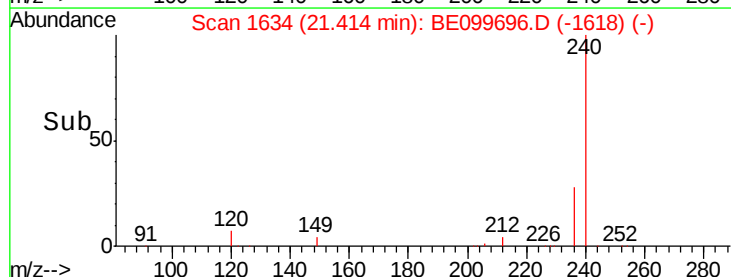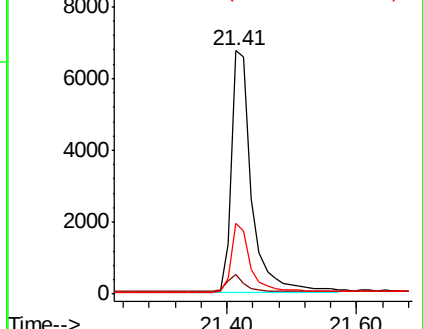

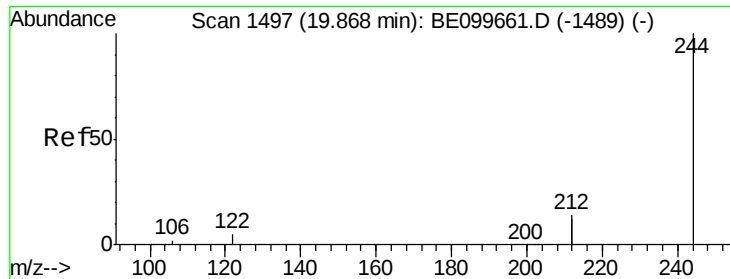

#29

Terphenyl-d14

Concen: 0.430 ng

RT: 19.86 min Scan# 1496

Delta R.T. -0.01 min

Lab File: BE099696.D

Acq: 21 May 2019 19:22

Instrument :

BNA_E

ClientSampleId :

PB119824BL


Tot Ion:244 Resp: 11348

Ion Ratio Lower Upper




244 100

212 30.2 22.5 33.7

122 6.8 4.3 6.5#

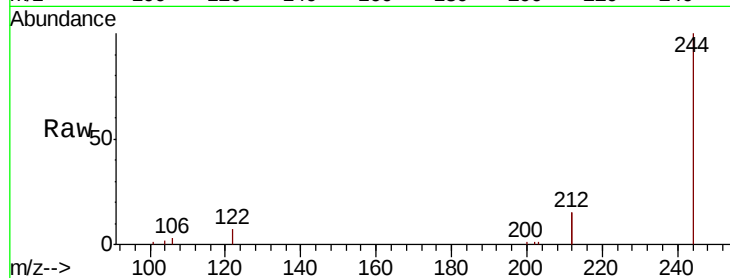

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

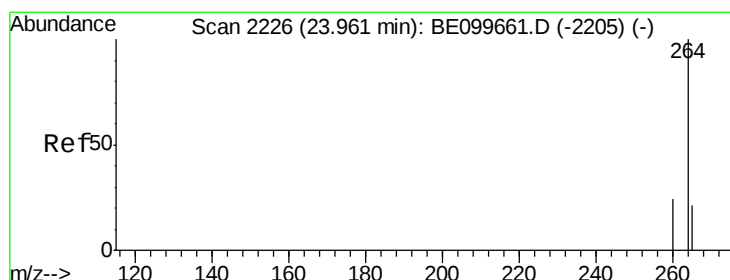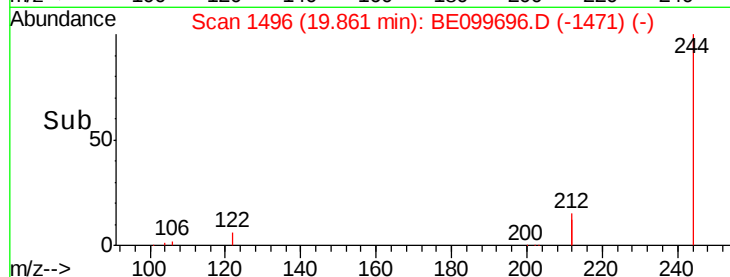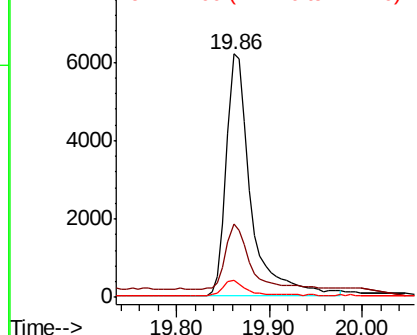

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.96 min Scan# 2225

Delta R.T. -0.00 min

Lab File: BE099696.D

Acq: 21 May 2019 19:22


Tgt Ion:264 Resp: 18091

Ion Ratio Lower Upper

264 100

260 24.9 19.6 29.4

265 25.8 19.1 28.7

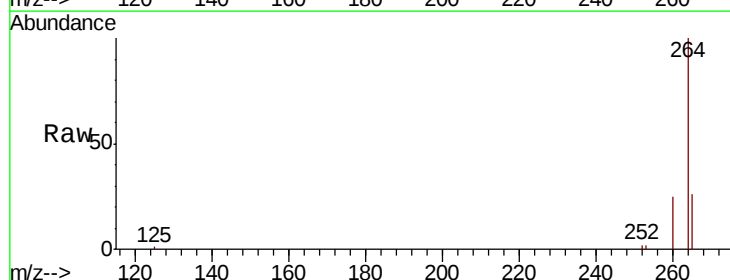

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

