


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE052119\
 Data File : BE099685.D
 Acq On : 21 May 2019 8:18
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE052019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 20 19:29:40 2019

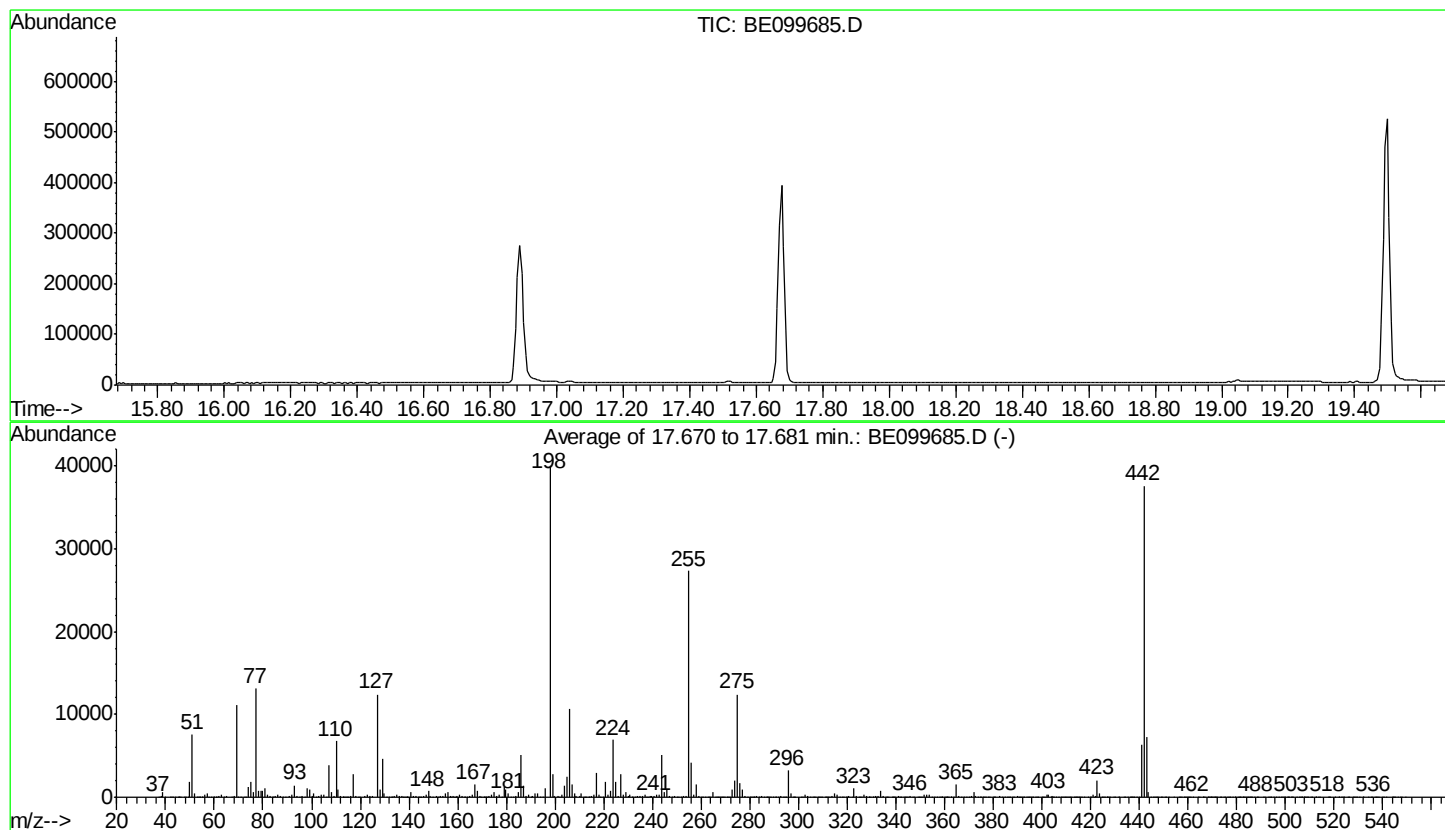

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2560

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.9	7557	PASS
68	69	0.00	2	1.5	163	PASS
69	198	0.00	100	27.7	11103	PASS
70	69	0.00	2	0.6	68	PASS
127	198	10	80	30.9	12374	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40021	PASS
199	198	5	9	6.9	2747	PASS
275	198	10	60	31.0	12417	PASS
365	198	1	100	3.9	1543	PASS
441	198	0.01	100	16.0	6385	PASS
442	198	50	100	93.9	37578	PASS
443	442	15	24	19.4	7284	PASS