


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE052219\
 Data File : BE099712.D
 Acq On : 22 May 2019 9:30
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE052019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 20 19:29:40 2019

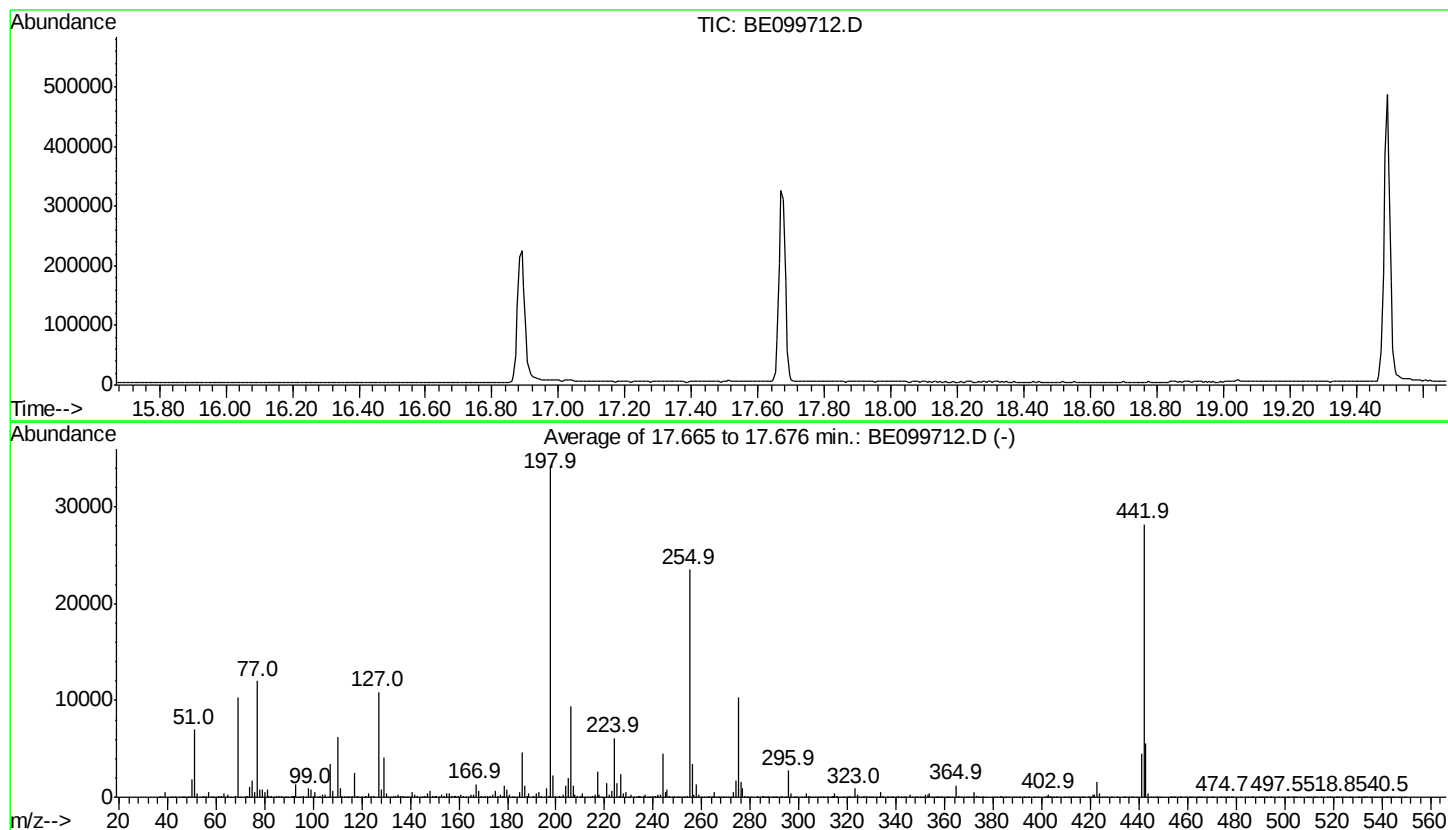

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.3	6957	PASS
68	69	0.00	2	1.8	185	PASS
69	198	0.00	100	30.0	10294	PASS
70	69	0.00	2	0.3	34	PASS
127	198	10	80	31.8	10886	PASS
197	198	0.00	2	0.2	76	PASS
198	198	100	100	100.0	34263	PASS
199	198	5	9	6.8	2317	PASS
275	198	10	60	30.3	10376	PASS
365	198	1	100	3.6	1244	PASS
441	198	0.01	100	13.3	4565	PASS
442	198	50	100	82.4	28243	PASS
443	442	15	24	19.6	5527	PASS