


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE052419\
Data File : BE099735.D
Acq On : 24 May 2019 10:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE052019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 20 19:29:40 2019

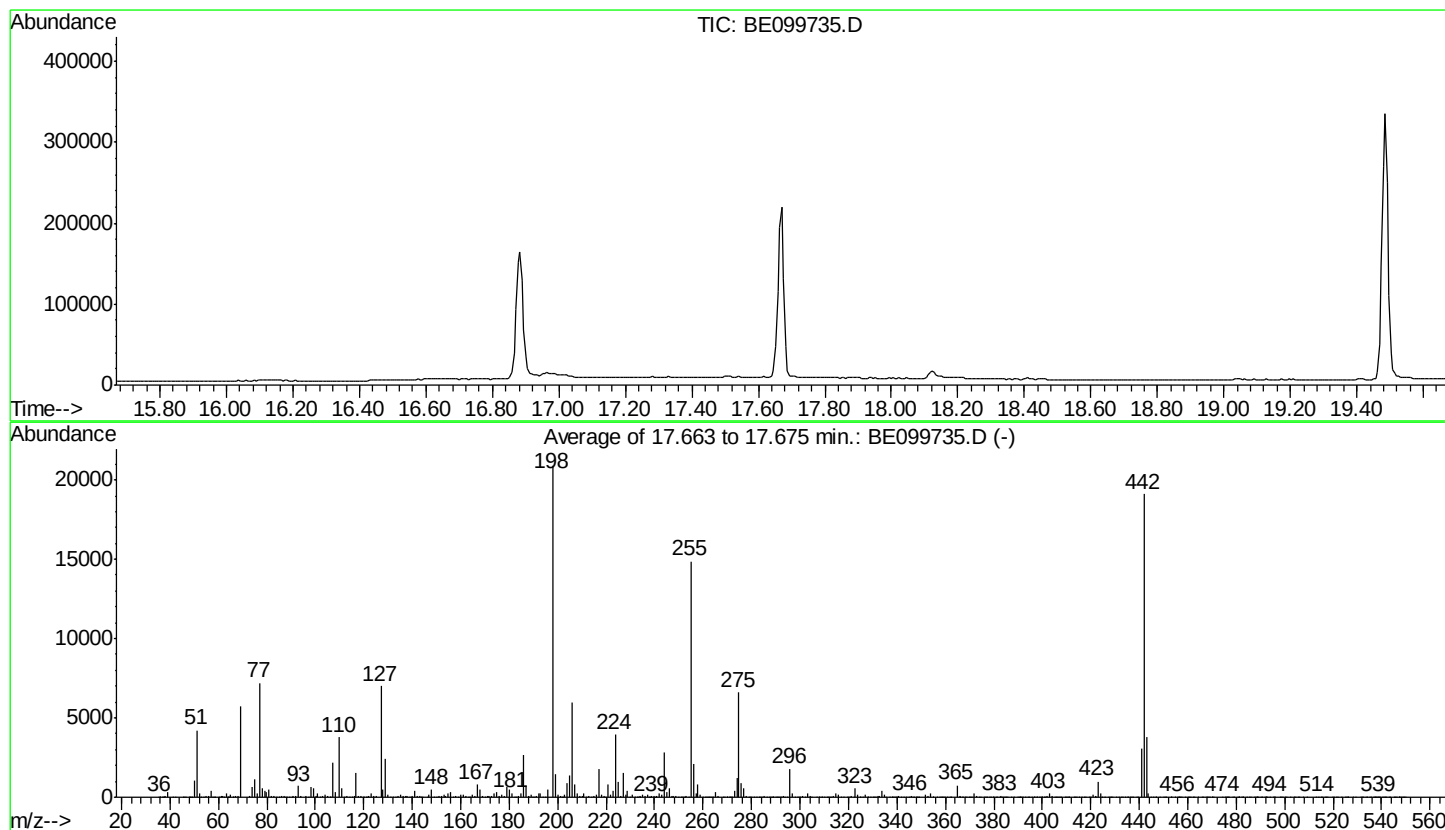

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.1	4202	PASS
68	69	0.00	2	1.2	66	PASS
69	198	0.00	100	27.4	5723	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.5	6992	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20899	PASS
199	198	5	9	6.9	1439	PASS
275	198	10	60	31.7	6615	PASS
365	198	1	100	3.6	743	PASS
441	198	0.01	100	14.6	3044	PASS
442	198	50	100	91.5	19117	PASS
443	442	15	24	19.7	3770	PASS