


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE060319\
Data File : BE099783.D
Acq On : 3 Jun 2019 13:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE052019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 20 19:29:40 2019

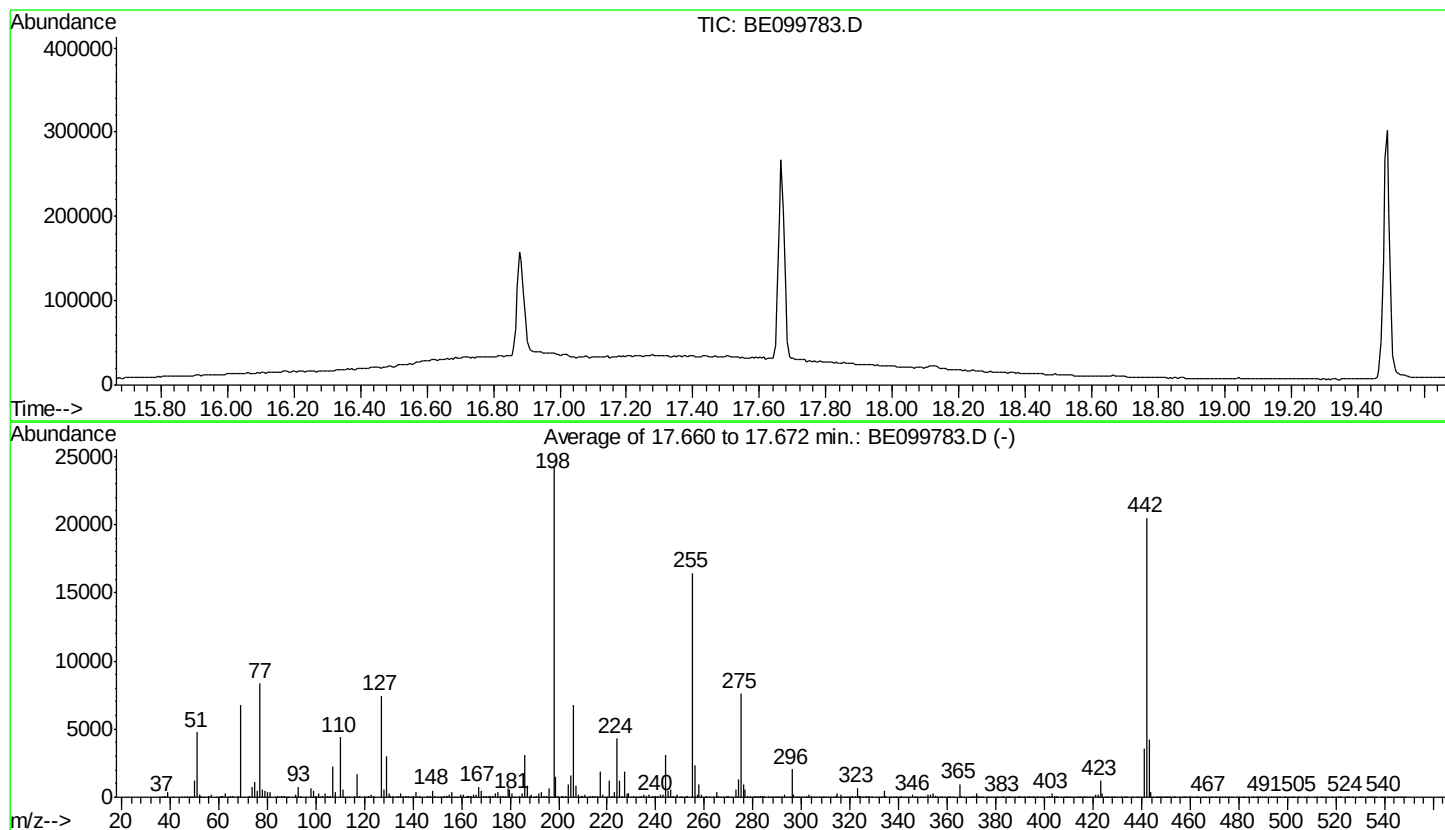

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.7	4786	PASS
68	69	0.00	2	1.7	112	PASS
69	198	0.00	100	27.7	6748	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	30.5	7419	PASS
197	198	0.00	2	0.2	47	PASS
198	198	100	100	100.0	24327	PASS
199	198	5	9	6.3	1536	PASS
275	198	10	60	31.1	7567	PASS
365	198	1	100	3.9	941	PASS
441	198	0.01	100	14.5	3525	PASS
442	198	50	100	84.3	20501	PASS
443	442	15	24	20.8	4258	PASS