


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE060419\
 Data File : BE099791.D
 Acq On : 4 Jun 2019 8:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE052019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 20 19:29:40 2019

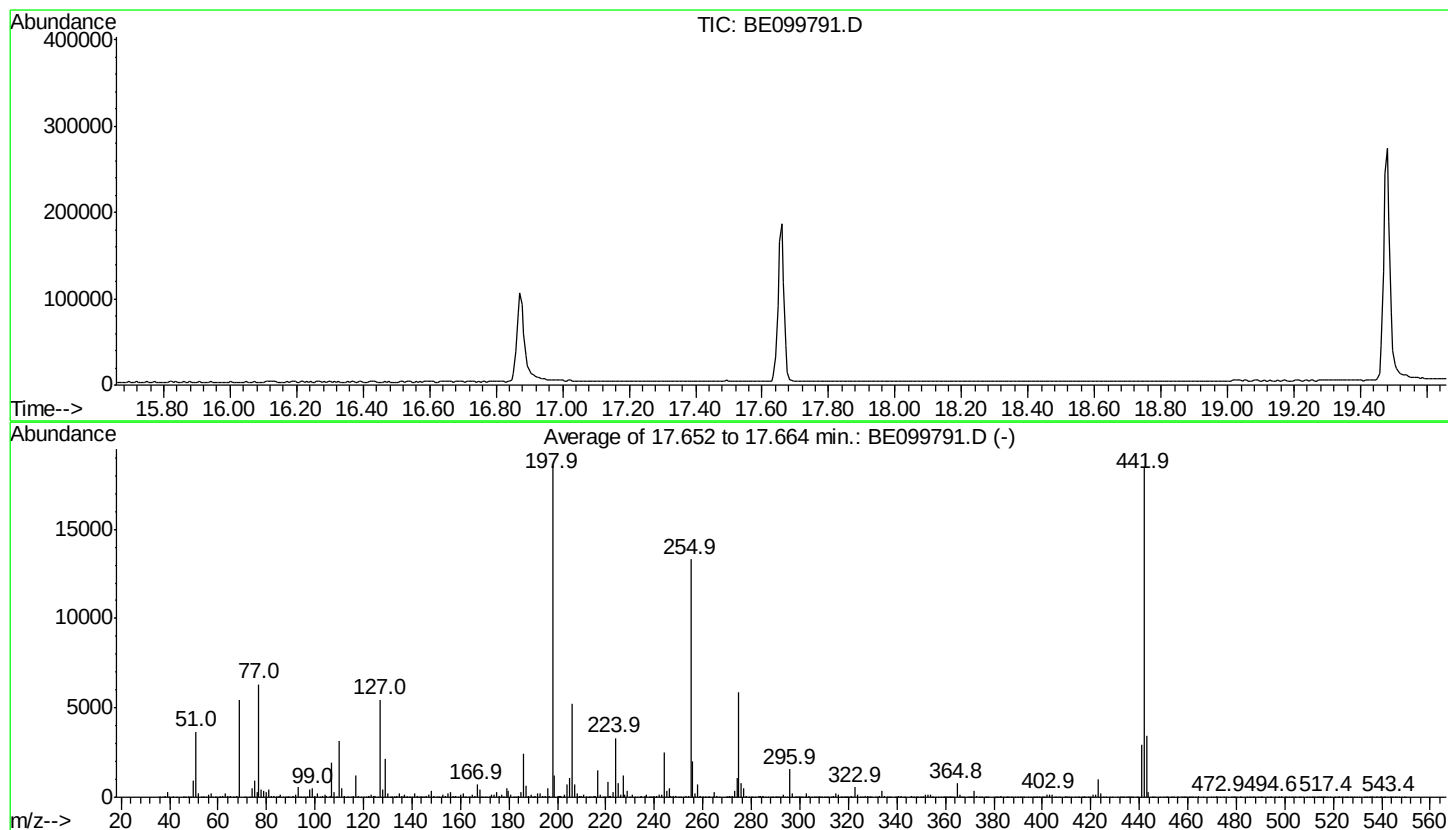

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.8	3668	PASS
68	69	0.00	2	1.9	104	PASS
69	198	0.00	100	29.2	5418	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	29.5	5479	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18557	PASS
199	198	5	9	6.5	1206	PASS
275	198	10	60	31.6	5868	PASS
365	198	1	100	4.1	766	PASS
441	198	0.01	100	15.8	2937	PASS
442	198	50	100	99.5	18457	PASS
443	442	15	24	18.5	3409	PASS