


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE060619\
 Data File : BE099813.D
 Acq On : 6 Jun 2019 7:50
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 05 14:35:58 2019

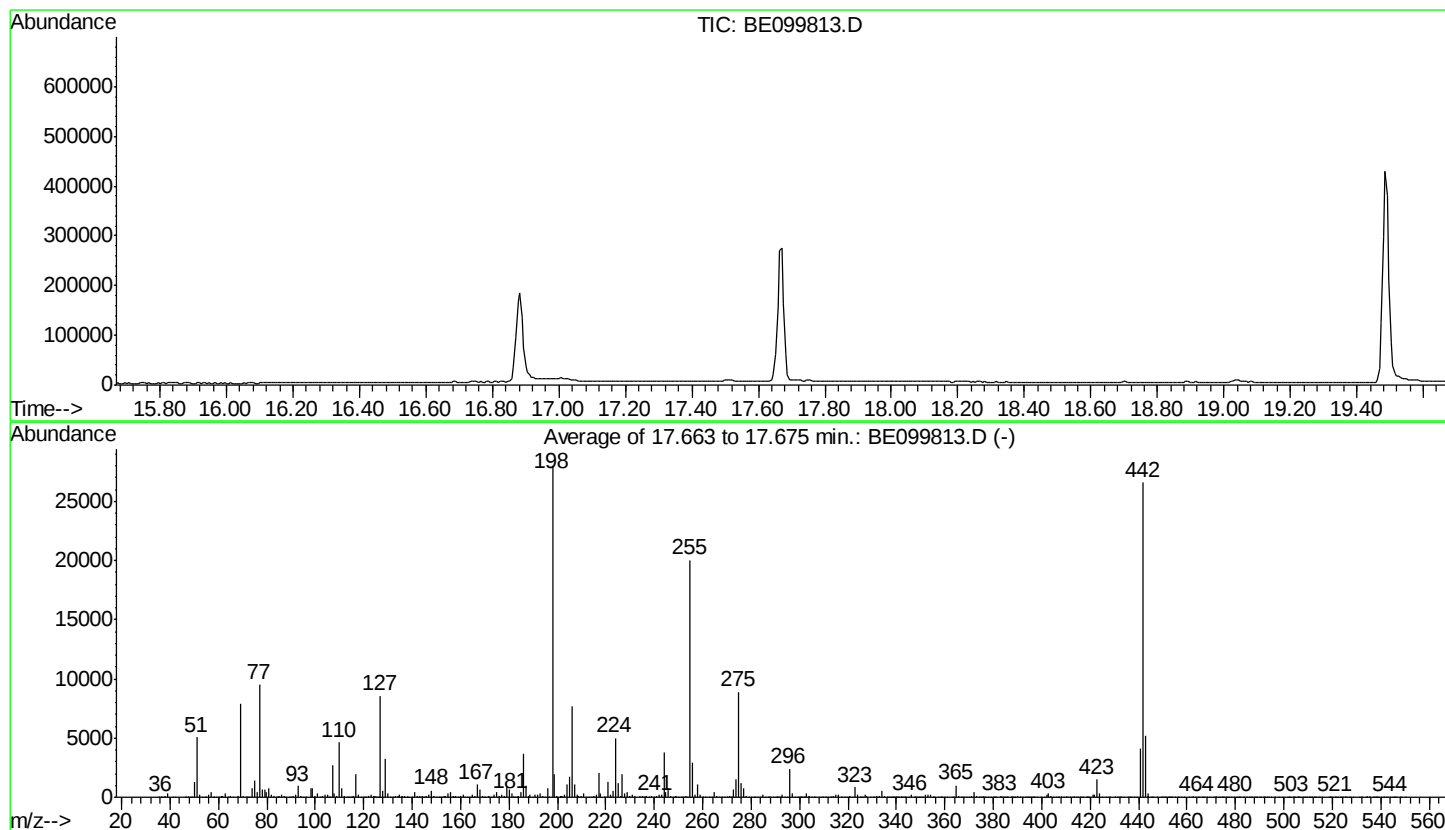

AutoFind: Scans 2566, 2567, 2568; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.0	5054	PASS
68	69	0.00	2	0.9	71	PASS
69	198	0.00	100	28.3	7912	PASS
70	69	0.00	2	1.3	101	PASS
127	198	10	80	30.6	8573	PASS
197	198	0.00	2	0.0	9	PASS
198	198	100	100	100.0	28007	PASS
199	198	5	9	6.8	1910	PASS
275	198	10	60	31.8	8898	PASS
365	198	1	100	3.5	988	PASS
441	198	0.01	100	14.8	4141	PASS
442	198	50	100	94.8	26563	PASS
443	442	15	24	19.5	5171	PASS