


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE060619\
 Data File : BE099825.D
 Acq On : 6 Jun 2019 17:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 05 14:35:58 2019

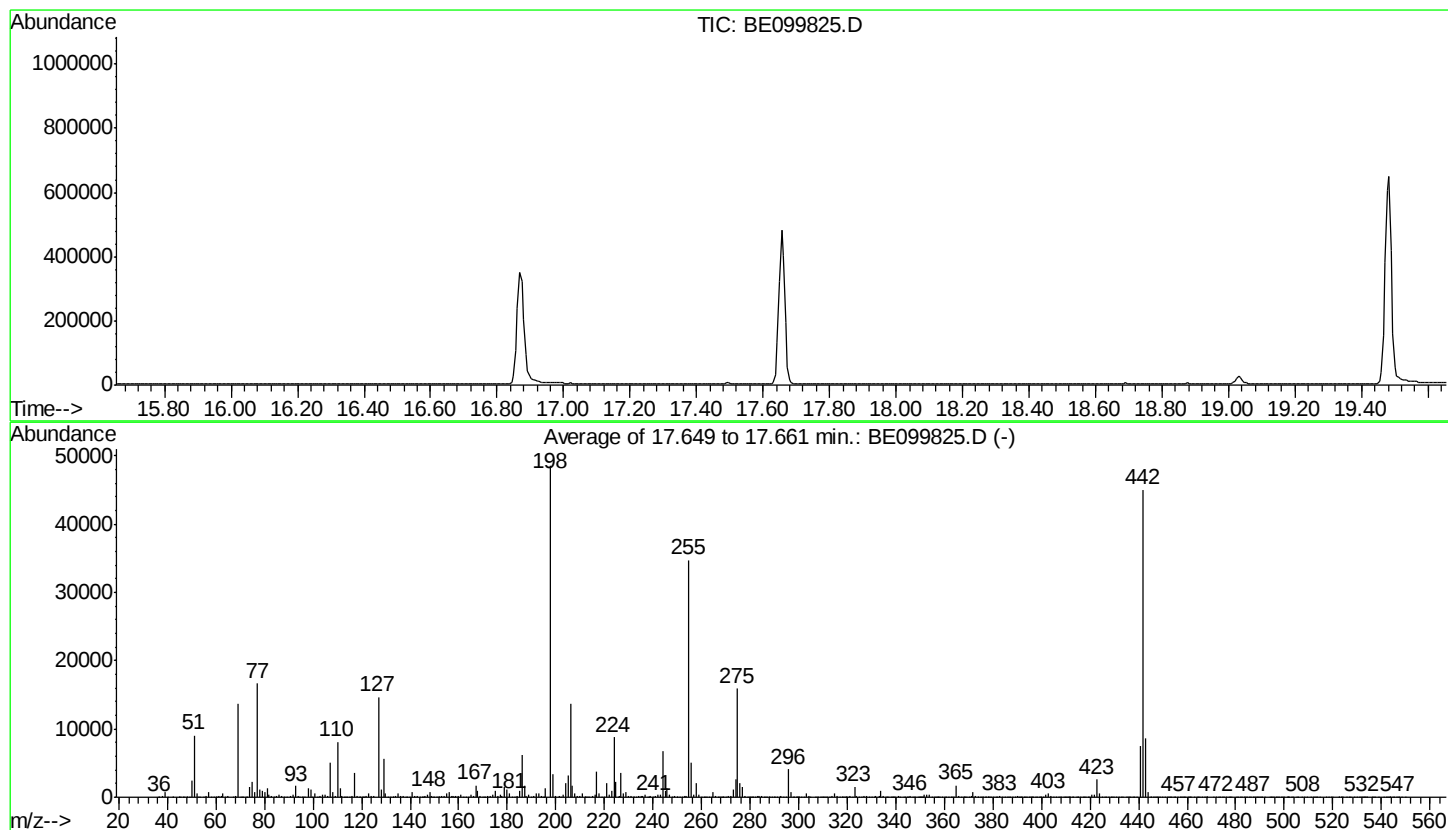

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.6	9022	PASS
68	69	0.00	2	0.9	124	PASS
69	198	0.00	100	28.0	13617	PASS
70	69	0.00	2	0.4	59	PASS
127	198	10	80	30.3	14699	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48554	PASS
199	198	5	9	6.9	3361	PASS
275	198	10	60	32.8	15914	PASS
365	198	1	100	3.5	1711	PASS
441	198	0.01	100	15.4	7470	PASS
442	198	50	100	92.7	45026	PASS
443	442	15	24	19.2	8665	PASS