


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE060719\
 Data File : BE099844.D
 Acq On : 7 Jun 2019 9:45
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 07 15:25:21 2019

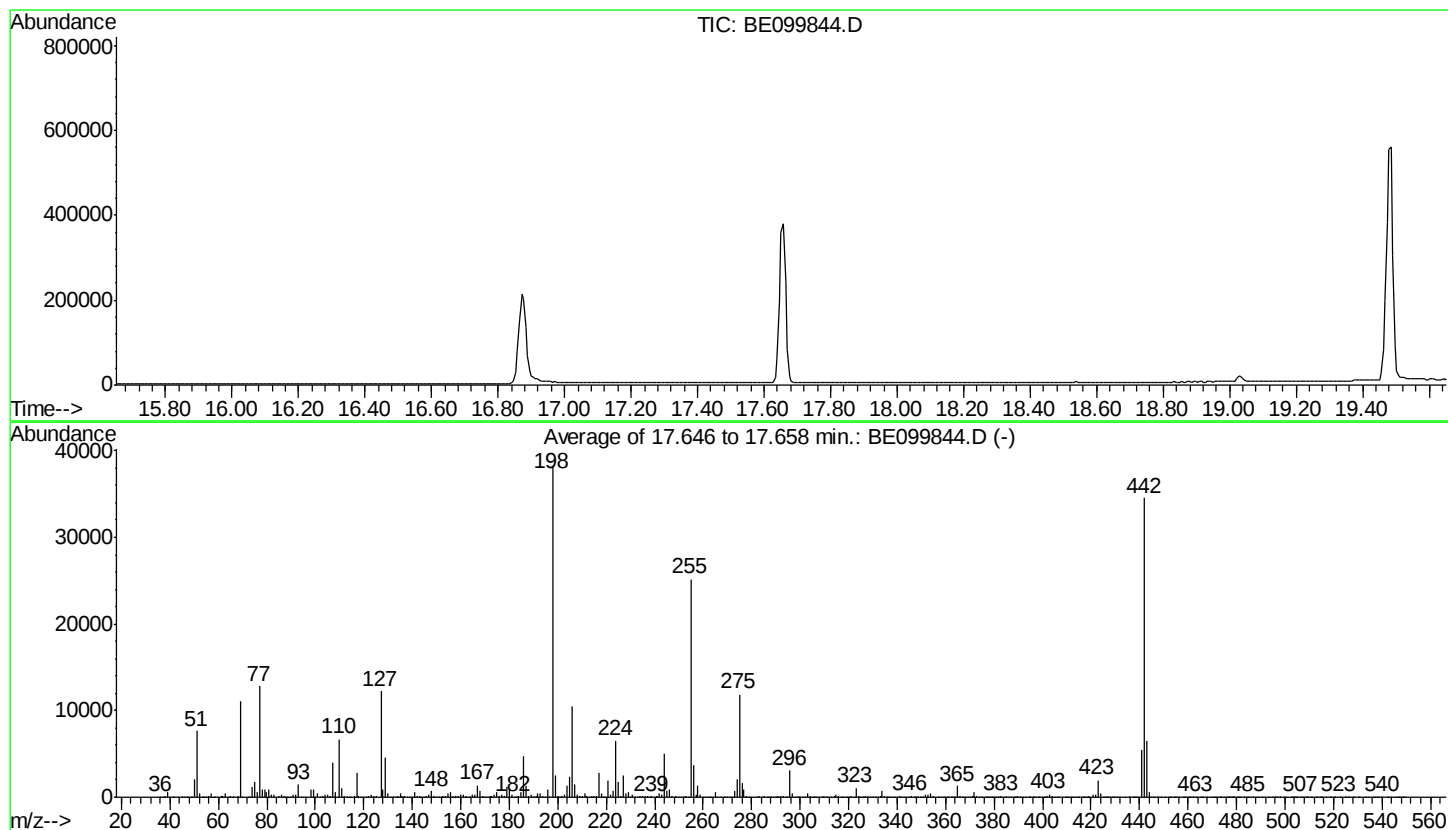

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.9	7621	PASS
68	69	0.00	2	1.3	139	PASS
69	198	0.00	100	28.8	11041	PASS
70	69	0.00	2	0.4	40	PASS
127	198	10	80	32.0	12251	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38278	PASS
199	198	5	9	6.7	2582	PASS
275	198	10	60	31.0	11849	PASS
365	198	1	100	3.4	1297	PASS
441	198	0.01	100	14.2	5446	PASS
442	198	50	100	90.2	34533	PASS
443	442	15	24	18.9	6528	PASS