


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE060719\
 Data File : BE099854.D
 Acq On : 7 Jun 2019 16:04
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 07 15:25:21 2019

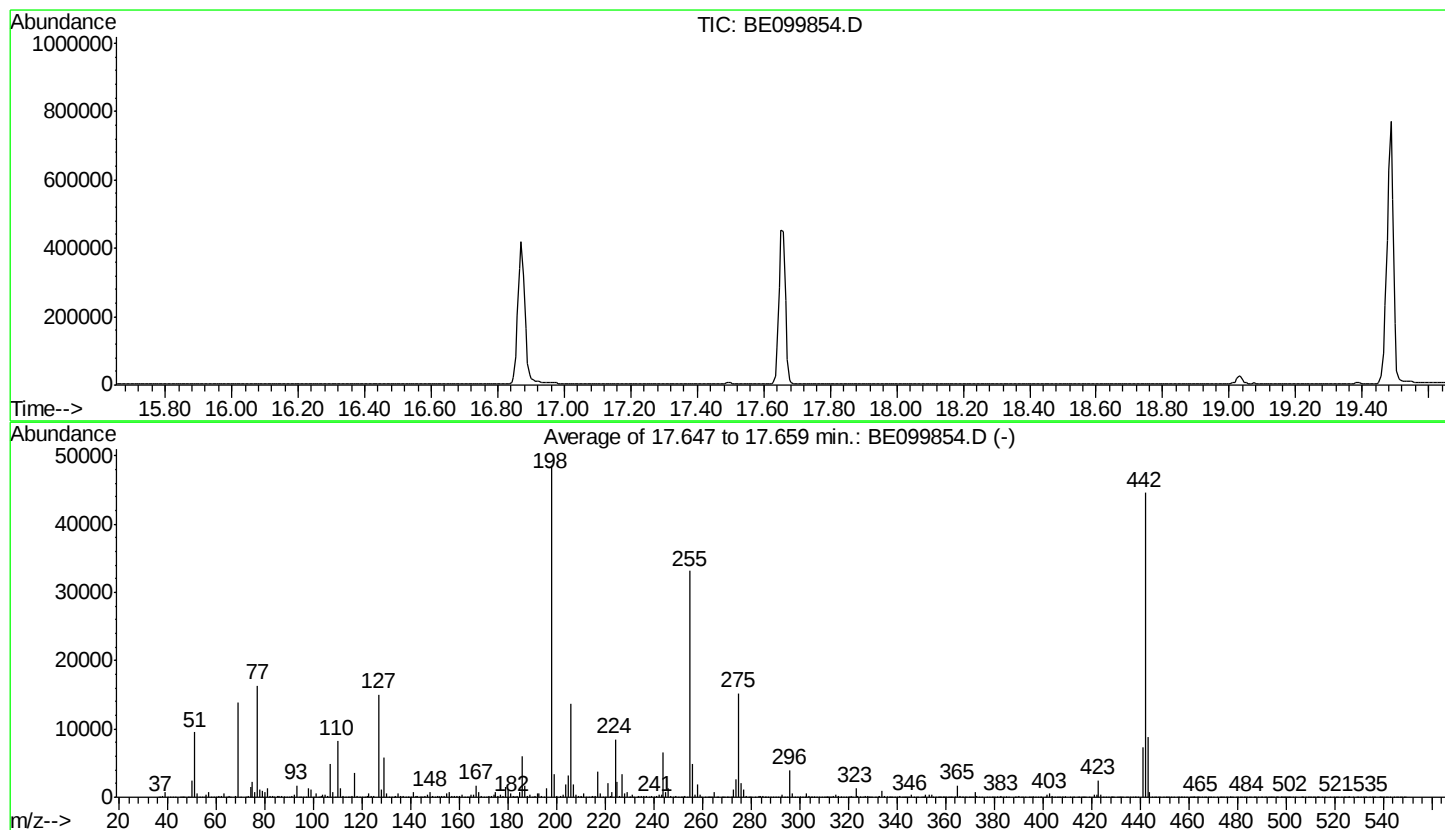

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.6	9495	PASS
68	69	0.00	2	0.9	124	PASS
69	198	0.00	100	28.7	13911	PASS
70	69	0.00	2	0.5	69	PASS
127	198	10	80	31.0	15038	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48543	PASS
199	198	5	9	7.0	3402	PASS
275	198	10	60	31.3	15203	PASS
365	198	1	100	3.5	1694	PASS
441	198	0.01	100	15.1	7347	PASS
442	198	50	100	91.7	44522	PASS
443	442	15	24	19.9	8865	PASS