


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE060719\
 Data File : BE099872.D
 Acq On : 8 Jun 2019 5:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 07 15:25:21 2019

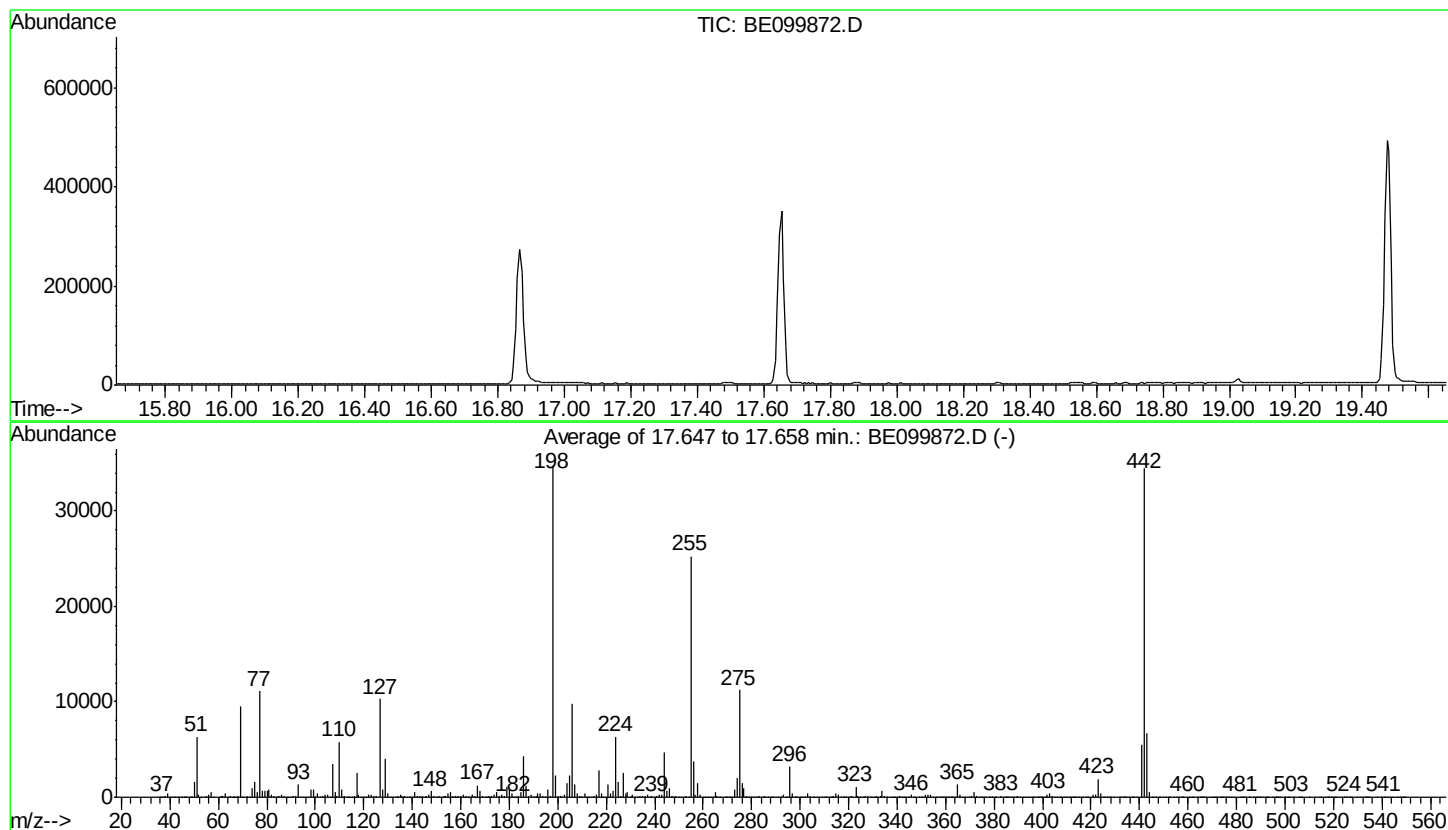

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.3	6355	PASS
68	69	0.00	2	1.5	139	PASS
69	198	0.00	100	27.5	9559	PASS
70	69	0.00	2	0.5	48	PASS
127	198	10	80	29.6	10296	PASS
197	198	0.00	2	0.3	89	PASS
198	198	100	100	100.0	34757	PASS
199	198	5	9	6.8	2349	PASS
275	198	10	60	32.4	11245	PASS
365	198	1	100	3.9	1341	PASS
441	198	0.01	100	15.8	5496	PASS
442	198	50	100	99.1	34456	PASS
443	442	15	24	19.4	6670	PASS