


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061019\
 Data File : BE099883.D
 Acq On : 10 Jun 2019 9:04
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 10 14:57:20 2019

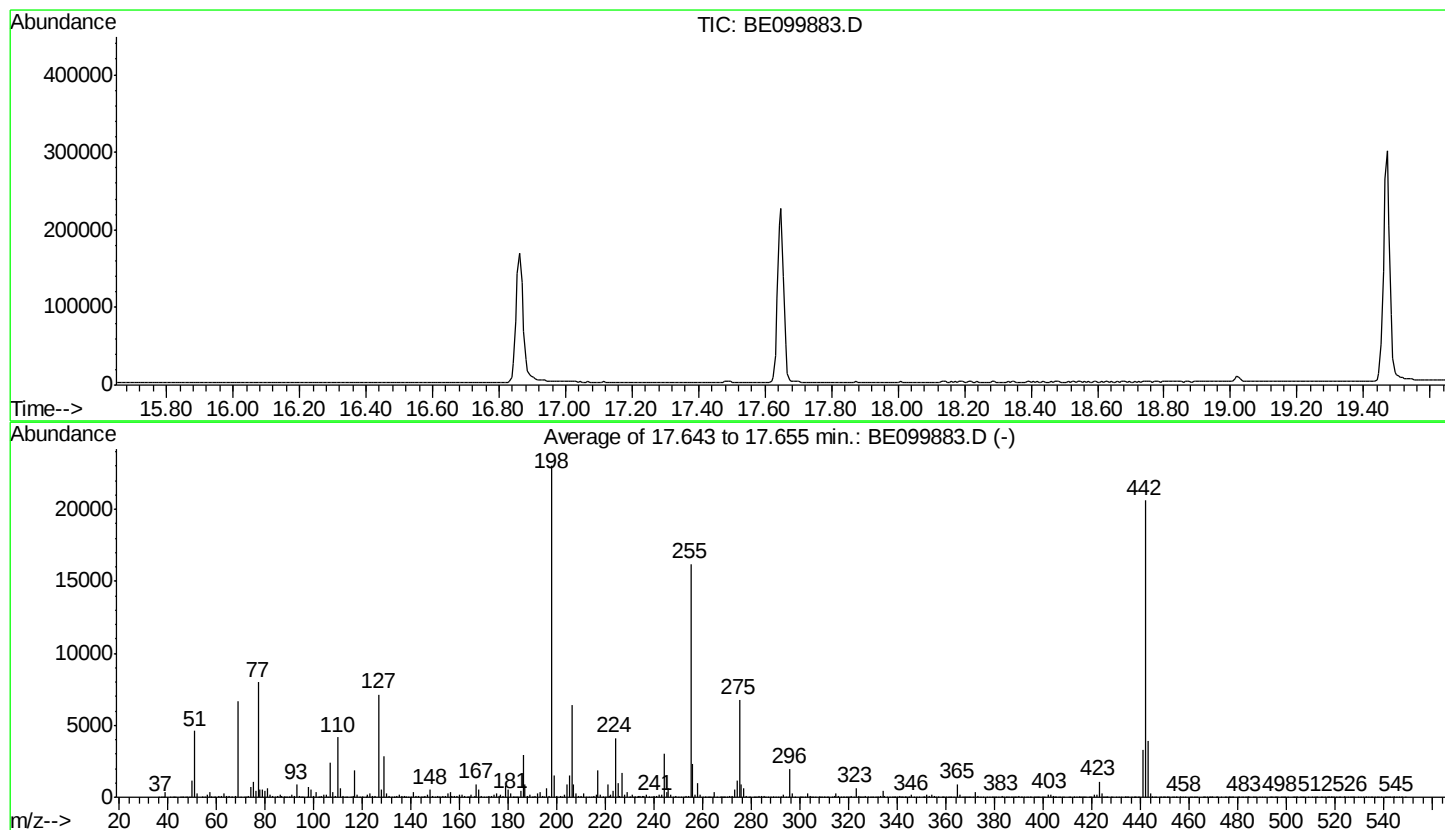

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.1	4623	PASS
68	69	0.00	2	1.1	74	PASS
69	198	0.00	100	28.9	6656	PASS
70	69	0.00	2	0.5	33	PASS
127	198	10	80	30.9	7131	PASS
197	198	0.00	2	0.5	111	PASS
198	198	100	100	100.0	23046	PASS
199	198	5	9	6.7	1543	PASS
275	198	10	60	29.5	6804	PASS
365	198	1	100	3.9	896	PASS
441	198	0.01	100	14.5	3334	PASS
442	198	50	100	89.5	20621	PASS
443	442	15	24	18.9	3904	PASS