


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE061019\
Data File : BE099893.D
Acq On : 10 Jun 2019 16:52
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 10 14:57:20 2019

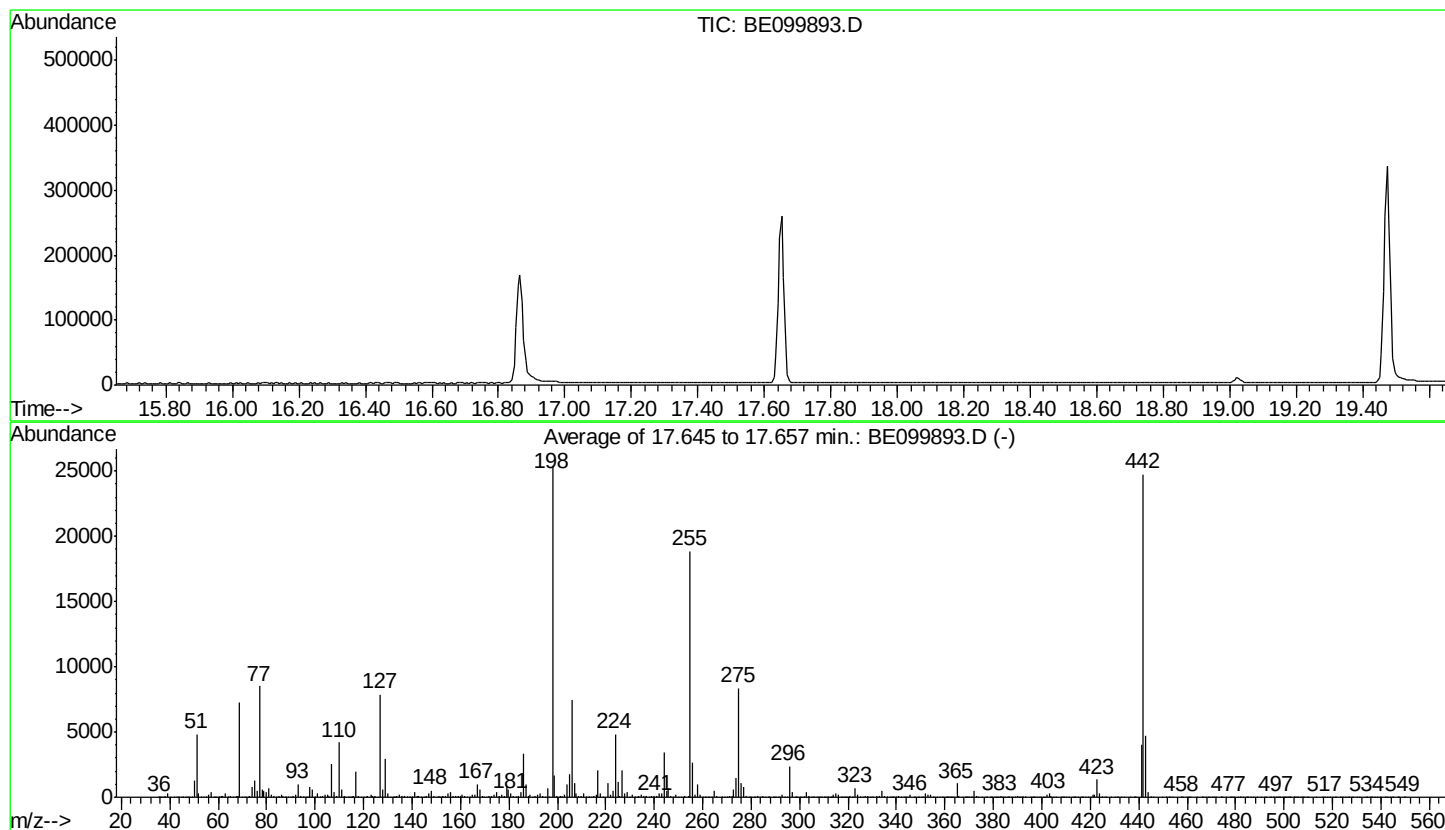

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.0	4823	PASS
68	69	0.00	2	0.9	62	PASS
69	198	0.00	100	28.6	7260	PASS
70	69	0.00	2	0.6	44	PASS
127	198	10	80	31.0	7877	PASS
197	198	0.00	2	0.1	23	PASS
198	198	100	100	100.0	25423	PASS
199	198	5	9	6.5	1659	PASS
275	198	10	60	33.0	8386	PASS
365	198	1	100	4.2	1057	PASS
441	198	0.01	100	15.8	4020	PASS
442	198	50	100	97.4	24750	PASS
443	442	15	24	19.2	4755	PASS